




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061722\  
 Data File : VV026390.D  
 Acq On : 17 Jun 2022 19:15  
 Operator : SY/MD  
 Sample : N3318-12 5X  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BGJ66

Manual IntegrationsAPPROVED

Quant Time: Jun 18 01:16:59 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR061522WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 18 01:02:22 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022  
 Supervised By :Mahesh Dadoda 06/20/2022

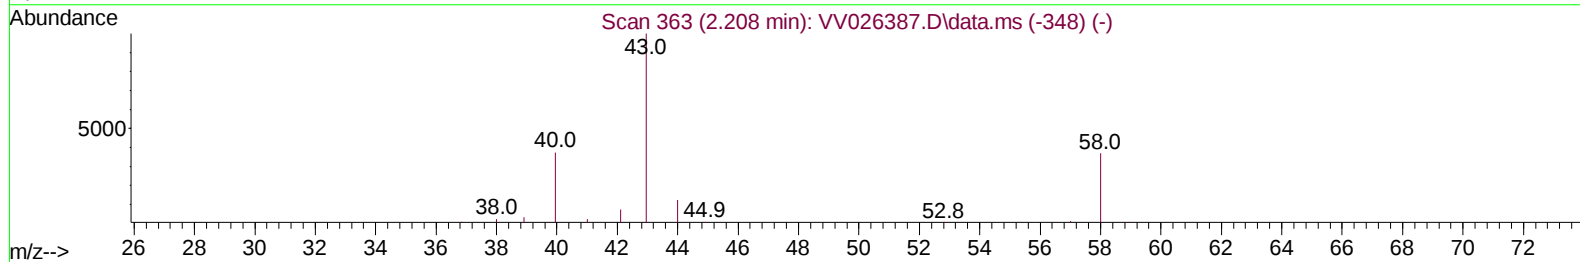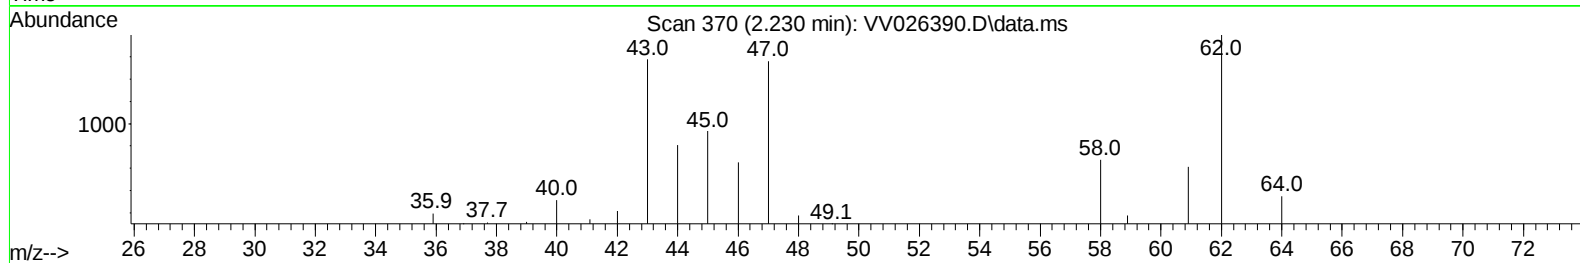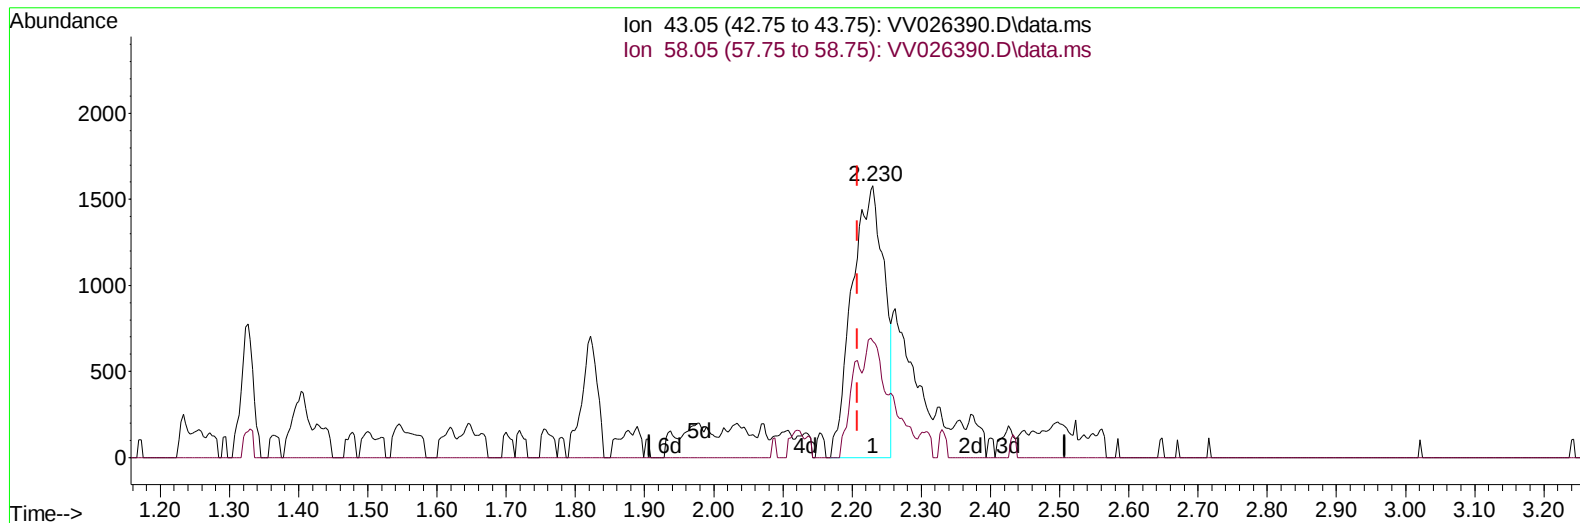

TIC: VV026390.D\data.ms

(13) Acetone (T)

2.230min (+ 0.022) 4.59 ug/L

response 5082

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 30.00  | 35.81  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061722\  
 Data File : VV026390.D  
 Acq On : 17 Jun 2022 19:15  
 Operator : SY/MD  
 Sample : N3318-12 5X  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BGJ66

Manual IntegrationsAPPROVED

Quant Time: Jun 18 01:16:59 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR061522WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 18 01:02:22 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022  
 Supervised By :Mahesh Dadoda 06/20/2022

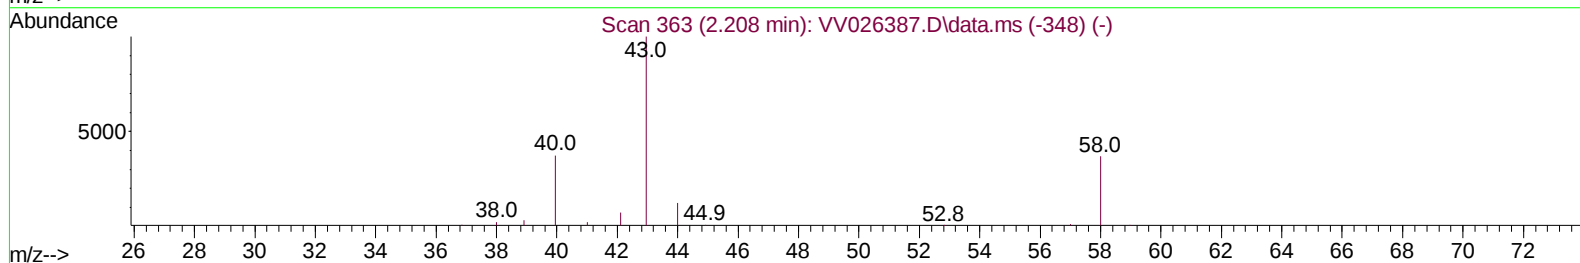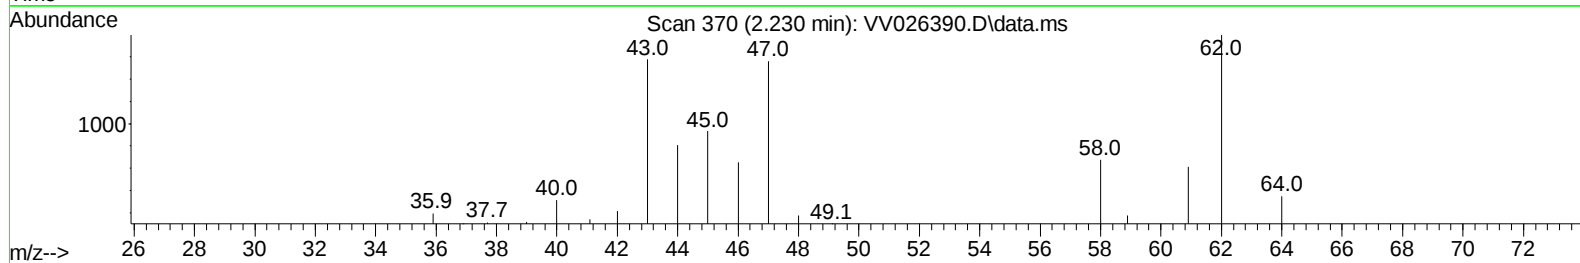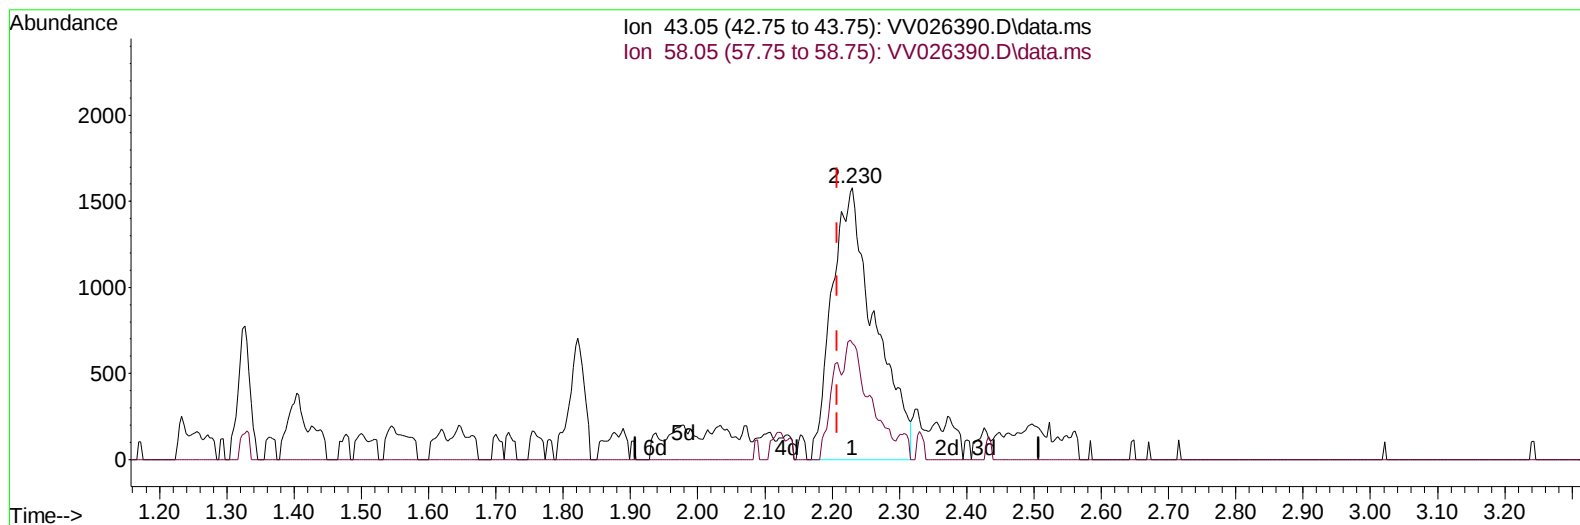

TIC: VV026390.D\data.ms

(13) Acetone (T)

2.230min (+ 0.022) 6.32 ug/L m

response 6991

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 30.00  | 26.03  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061722\  
 Data File : VV026390.D  
 Acq On : 17 Jun 2022 19:15  
 Operator : SY/MD  
 Sample : N3318-12 5X  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BGJ66

Manual IntegrationsAPPROVED

Quant Time: Jun 18 01:16:59 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR061522WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 18 01:02:22 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022  
 Supervised By :Mahesh Dadoda 06/20/2022

| Compound                      | R.T.     | QIon  | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|----------|-------|----------|--------|----------|----------|
| -----                         |          |       |          |        |          |          |
| Internal Standards            |          |       |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.629    | 114   | 168458   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.854    | 117   | 162976   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249   | 152   | 67073    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |          |       |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.323    | 65    | 55123    | 3.767  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 40 | - 130 | Recovery | =      | 75.400%  |          |
| 7) Chloroethane-d5            | 1.584    | 69    | 48395    | 4.207  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 130 | Recovery | =      | 84.200%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.124    | 63    | 80091    | 3.188  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 125 | Recovery | =      | 63.800%  |          |
| 20) 2-Butanone-d5             | 3.925    | 46    | 82007    | 57.439 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 40 | - 130 | Recovery | =      | 114.880% |          |
| 24) Chloroform-d              | 4.365    | 84    | 103252   | 4.815  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 | Recovery | =      | 96.200%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.047    | 65    | 44166    | 4.868  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 | Recovery | =      | 97.400%  |          |
| 32) Benzene-d6                | 5.063    | 84    | 190247   | 4.366  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 | Recovery | =      | 87.400%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.079    | 67    | 61145    | 4.808  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 140 | Recovery | =      | 96.200%  |          |
| 41) Toluene-d8                | 7.320    | 98    | 145384   | 3.659  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 | Recovery | =      | 73.200%  |          |
| 43) trans-1,3-Dichloroprop... | 7.632    | 79    | 11700    | 2.837  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 55 | - 130 | Recovery | =      | 56.800%  |          |
| 46) 2-Hexanone-d5             | 8.095    | 63    | 56723    | 45.538 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 45 | - 130 | Recovery | =      | 91.080%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217   | 84    | 40866    | 5.217  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 120 | Recovery | =      | 104.400% |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.625   | 152   | 50483    | 4.886  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 80 | - 120 | Recovery | =      | 97.800%  |          |
| Target Compounds              |          |       |          |        |          |          |
|                               |          |       |          |        | Qvalue   |          |
| 5) Vinyl chloride             | 1.330    | 62    | 21332    | 1.467  | ug/L #   | 55       |
| 12) 1,1-Dichloroethene        | 2.134    | 96    | 4944     | 0.465  | ug/L #   | 1        |
| 13) Acetone                   | 2.230    | 43    | 6991m    | 6.318  | ug/L     |          |
| 14) Carbon disulfide          | 2.317    | 76    | 2273     | 0.087  | ug/L     | 98       |
| 16) Methylene chloride        | 2.526    | 84    | 6902     | 0.508  | ug/L     | 95       |
| 18) trans-1,2-Dichloroethene  | 2.780    | 96    | 1053     | 0.102  | ug/L     | 91       |
| 19) 1,1-Dichloroethane        | 3.211    | 63    | 25745    | 1.308  | ug/L     | 97       |
| 22) cis-1,2-Dichloroethene    | 3.931    | 96    | 42728    | 4.091  | ug/L     | 100      |
| 34) Trichloroethene           | 5.924    | 95    | 16894    | 1.481  | ug/L     | 92       |
| 47) Tetrachloroethene         | 7.982    | 164   | 4376     | 0.518  | ug/L     | 91       |
| -----                         |          |       |          |        |          |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061722\  
Data File : VV026390.D  
Acq On : 17 Jun 2022 19:15  
Operator : SY/MD  
Sample : N3318-12 5X  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BGJ66

## Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/18/2022  
Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 18 01:16:59 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR061522WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 18 01:02:22 2022  
Response via : Initial Calibration

