




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026408.D
 Acq On : 18 Jun 2022 02:28
 Operator : SY/MD
 Sample : N3358-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4R7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 18 03:25:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

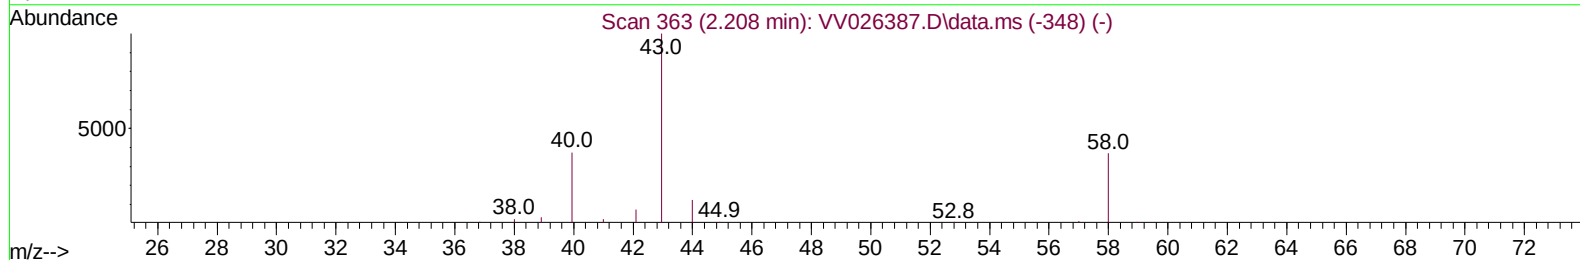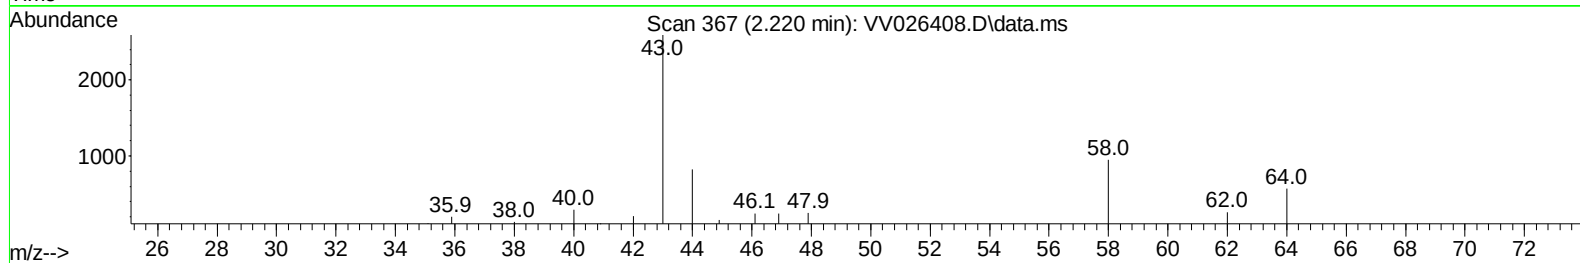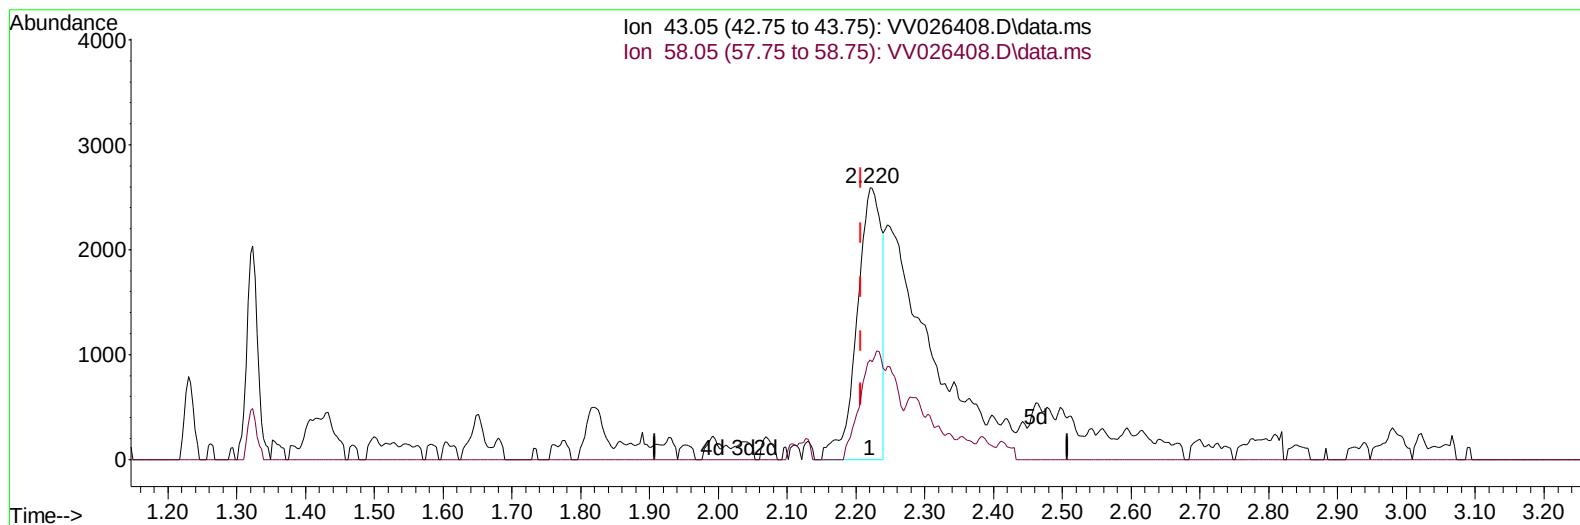

TIC: VV026408.D\data.ms

(13) Acetone (T)

2.220min (+ 0.013) 5.29 ug/L

response 6463

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	38.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026408.D
 Acq On : 18 Jun 2022 02:28
 Operator : SY/MD
 Sample : N3358-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4R7

Manual IntegrationsAPPROVED

Quant Time: Jun 18 03:25:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

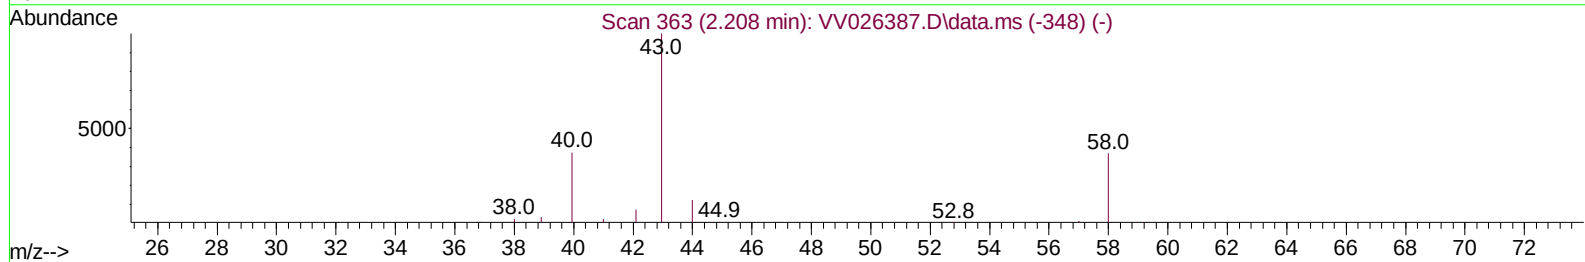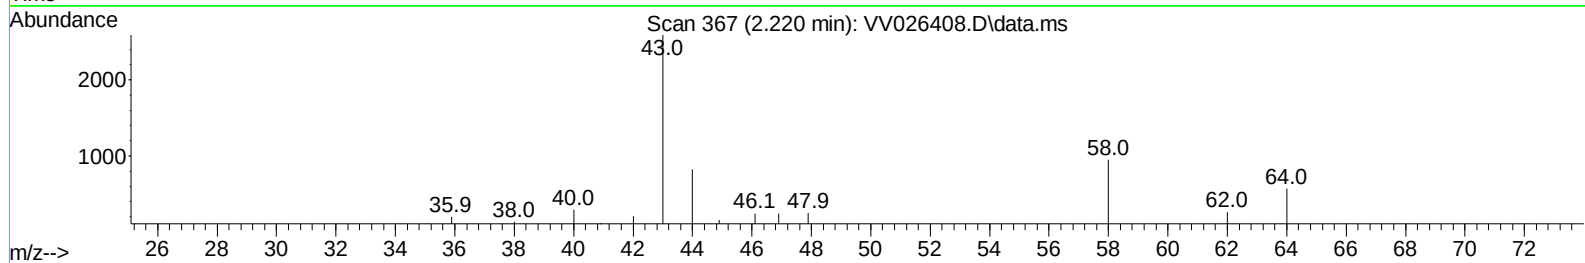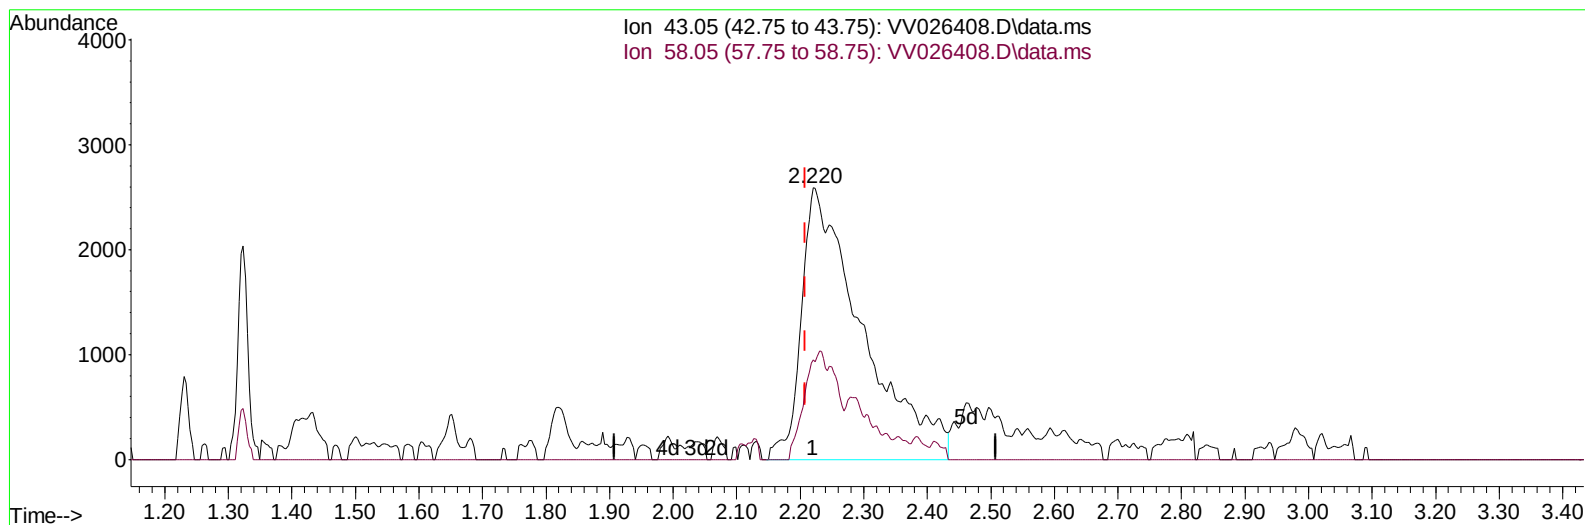

TIC: VV026408.D\data.ms

(13) Acetone (T)

2.220min (+ 0.013) 14.13 ug/L m

response 17244

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	30.00	14.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026408.D
 Acq On : 18 Jun 2022 02:28
 Operator : SY/MD
 Sample : N3358-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4R7

Manual IntegrationsAPPROVED

Quant Time: Jun 18 03:25:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/18/2022
 Supervised By :Mahesh Dadoda 06/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	185849	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	179532	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71480	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	46738	2.895	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	58.000%		
7) Chloroethane-d5	1.584	69	46197	3.640	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	72.800%		
11) 1,1-Dichloroethene-d2	2.121	63	68342	2.465	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	49.400%#		
20) 2-Butanone-d5	3.937	46	65608	41.653	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	83.300%		
24) Chloroform-d	4.362	84	106178	4.488	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.800%		
26) 1,2-Dichloroethane-d4	5.047	65	43590	4.355	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	87.000%		
32) Benzene-d6	5.063	84	187066	3.897	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	78.000%		
36) 1,2-Dichloropropane-d6	6.076	67	61240	4.372	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	87.400%		
41) Toluene-d8	7.320	98	140669	3.214	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	64.200%#		
43) trans-1,3-Dichloroprop...	7.632	79	11293	2.486	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	49.800%#		
46) 2-Hexanone-d5	8.095	63	55338	40.329	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	80.660%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40446	4.687	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	93.800%		
66) 1,2-Dichlorobenzene-d4	11.622	152	50777	4.612	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	92.200%		
Target Compounds						
					Qvalue	
13) Acetone	2.220	43	17244m	14.127	ug/L	
14) Carbon disulfide	2.310	76	22862	0.790	ug/L	99
42) Toluene	7.400	91	10159	0.210	ug/L	97
53) m,p-Xylene	9.146	106	1596	0.084	ug/L	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026408.D
Acq On : 18 Jun 2022 02:28
Operator : SY/MD
Sample : N3358-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4R7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/18/2022
Supervised By :Mahesh Dadoda 06/20/2022

Quant Time: Jun 18 03:25:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 18 01:02:22 2022
Response via : Initial Calibration

