

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026388.D
 Acq On : 17 Jun 2022 17:56
 Operator : SY/MD
 Sample : VV0617WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK378

Quant Time: Jun 18 01:04:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	183127	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	177357	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73051	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	55300	3.477	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	69.600%	
7) Chloroethane-d5	1.584	69	51394	4.109	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	82.200%	
11) 1,1-Dichloroethene-d2	2.121	63	82150	3.008	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.200%	
20) 2-Butanone-d5	3.915	46	94217	60.705	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	121.420%	
24) Chloroform-d	4.362	84	113930	4.887	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.043	65	48910	4.959	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.200%	
32) Benzene-d6	5.060	84	213717	4.507	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
36) 1,2-Dichloropropane-d6	6.076	67	67515	4.879	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.600%	
41) Toluene-d8	7.317	98	168037	3.887	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	77.800%	
43) trans-1,3-Dichloroprop...	7.629	79	13499	3.008	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	60.200%	
46) 2-Hexanone-d5	8.092	63	63805	47.070	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.140%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44665	5.239	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	58732	5.220	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.523	84	12314	0.834	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026388.D
Acq On : 17 Jun 2022 17:56
Operator : SY/MD
Sample : VV0617WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK378

Quant Time: Jun 18 01:04:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 18 01:02:22 2022
Response via : Initial Calibration

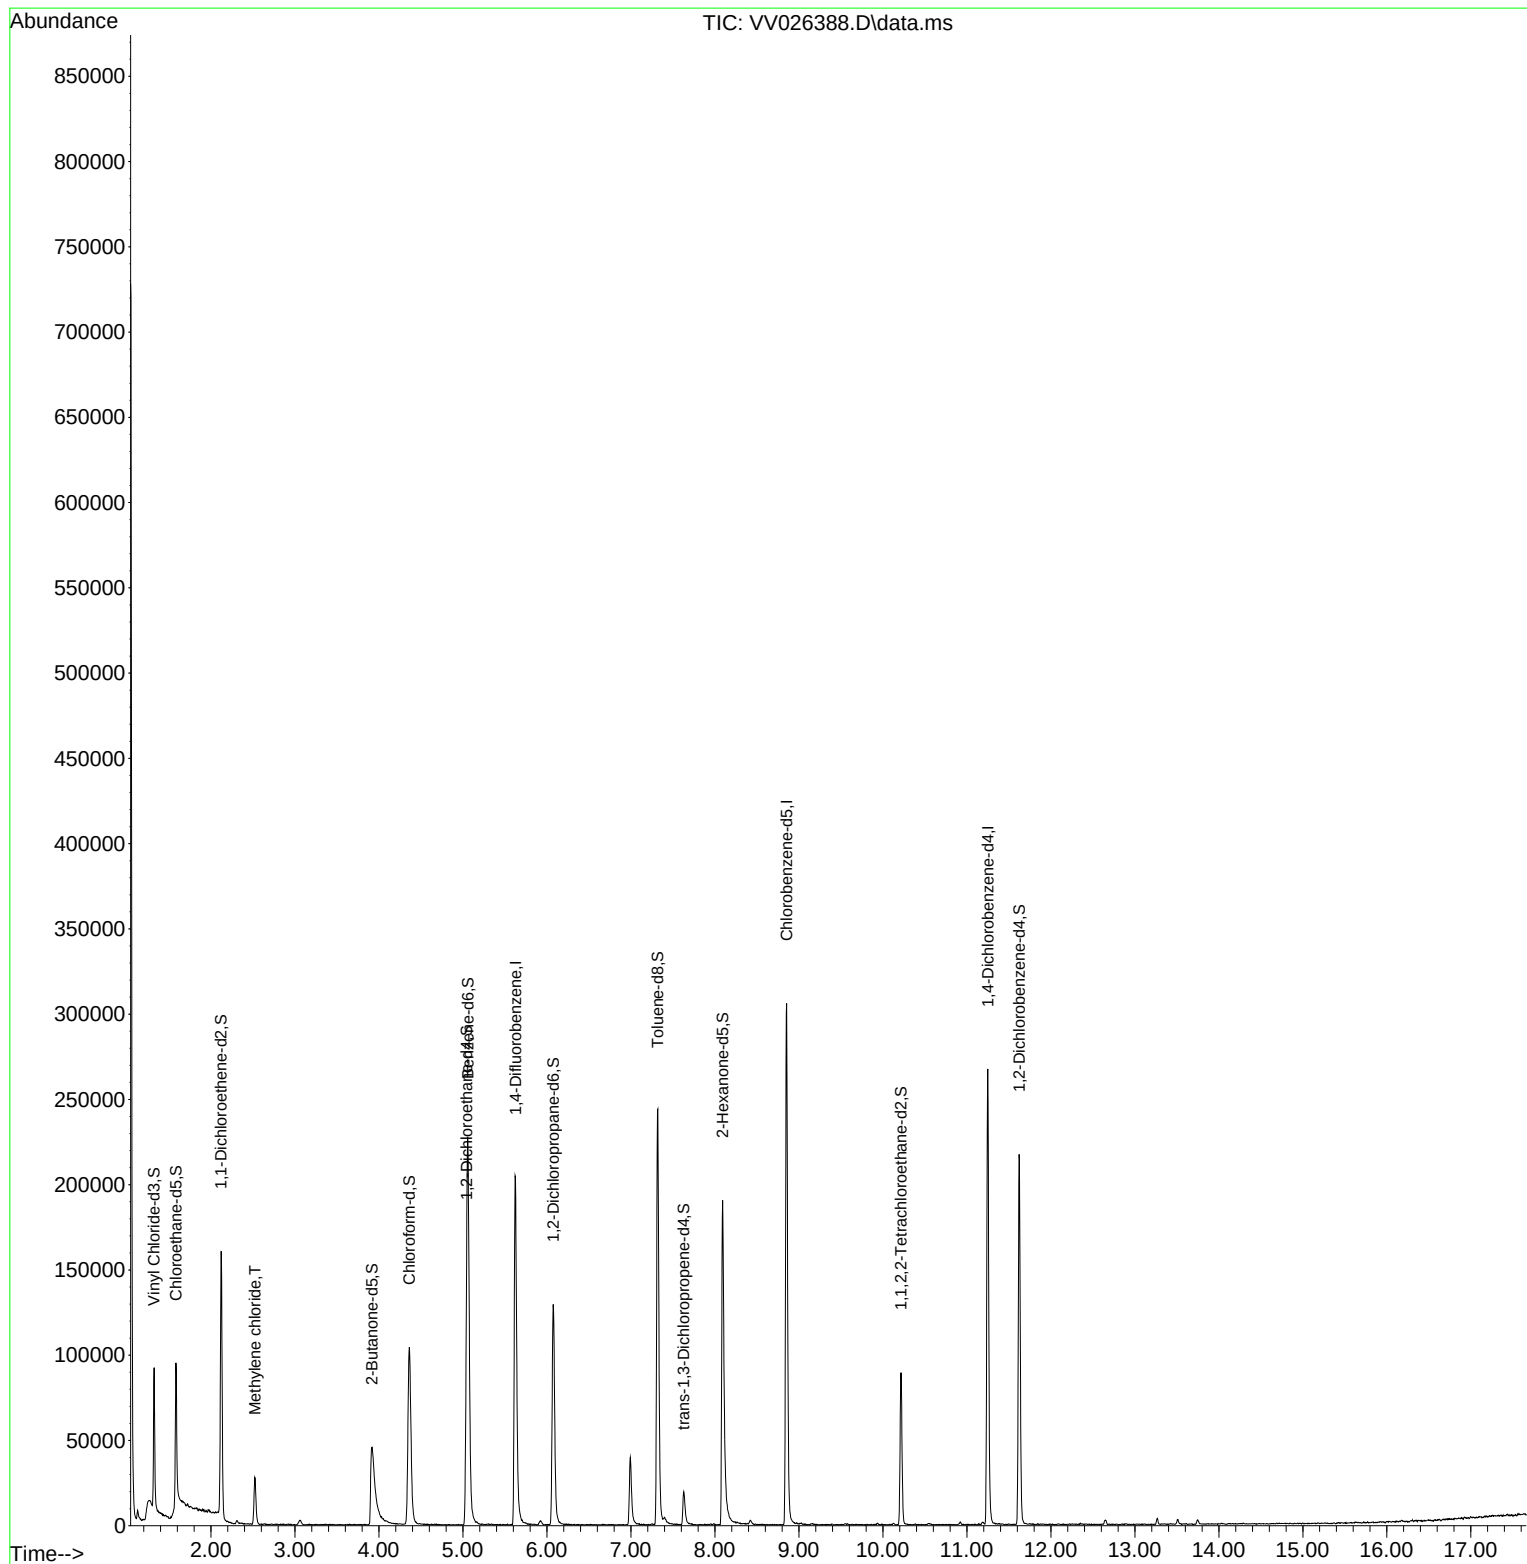

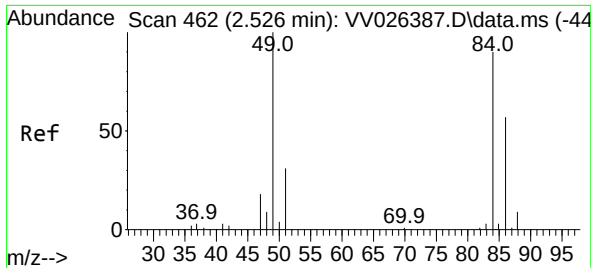

#16
Methylene chloride
Concen: 0.834 ug/L
RT: 2.523 min Scan# 4
Delta R.T. -0.003 min
Lab File: VV026388.D
Acq: 17 Jun 2022 17:56

Instrument :
MSVOA_V
ClientSampleId :
VBLK378

Tgt Ion: 84 Resp: 12314
Ion Ratio Lower Upper
84 100
86 61.8 44.0 81.8
49 105.3 77.3 143.7

