

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061722\
 Data File : VW026392.D
 Acq On : 17 Jun 2022 20:04
 Operator : SY/MD
 Sample : N3318-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 18 01:17:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	177881	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	170814	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70016	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	51217	3.315	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.200%
7) Chloroethane-d5	1.584	69	49384	4.065	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	2.124	63	75703	2.853	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.000%#
20) 2-Butanone-d5	3.924	46	87376	57.958	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.920%
24) Chloroform-d	4.365	84	111248	4.913	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.047	65	45597	4.759	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%
32) Benzene-d6	5.063	84	198562	4.348	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	6.079	67	63959	4.799	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.320	98	152091	3.652	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.000%
43) trans-1,3-Dichloroprop...	7.632	79	12246	2.833	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.600%
46) 2-Hexanone-d5	8.092	63	61461	47.077	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.160%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44556	5.427	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	54296	5.035	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%
Target Compounds						
16) Methylene chloride	2.526	84	6545	0.456	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026392.D
Acq On : 17 Jun 2022 20:04
Operator : SY/MD
Sample : N3318-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 18 01:17:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 18 01:02:22 2022
Response via : Initial Calibration

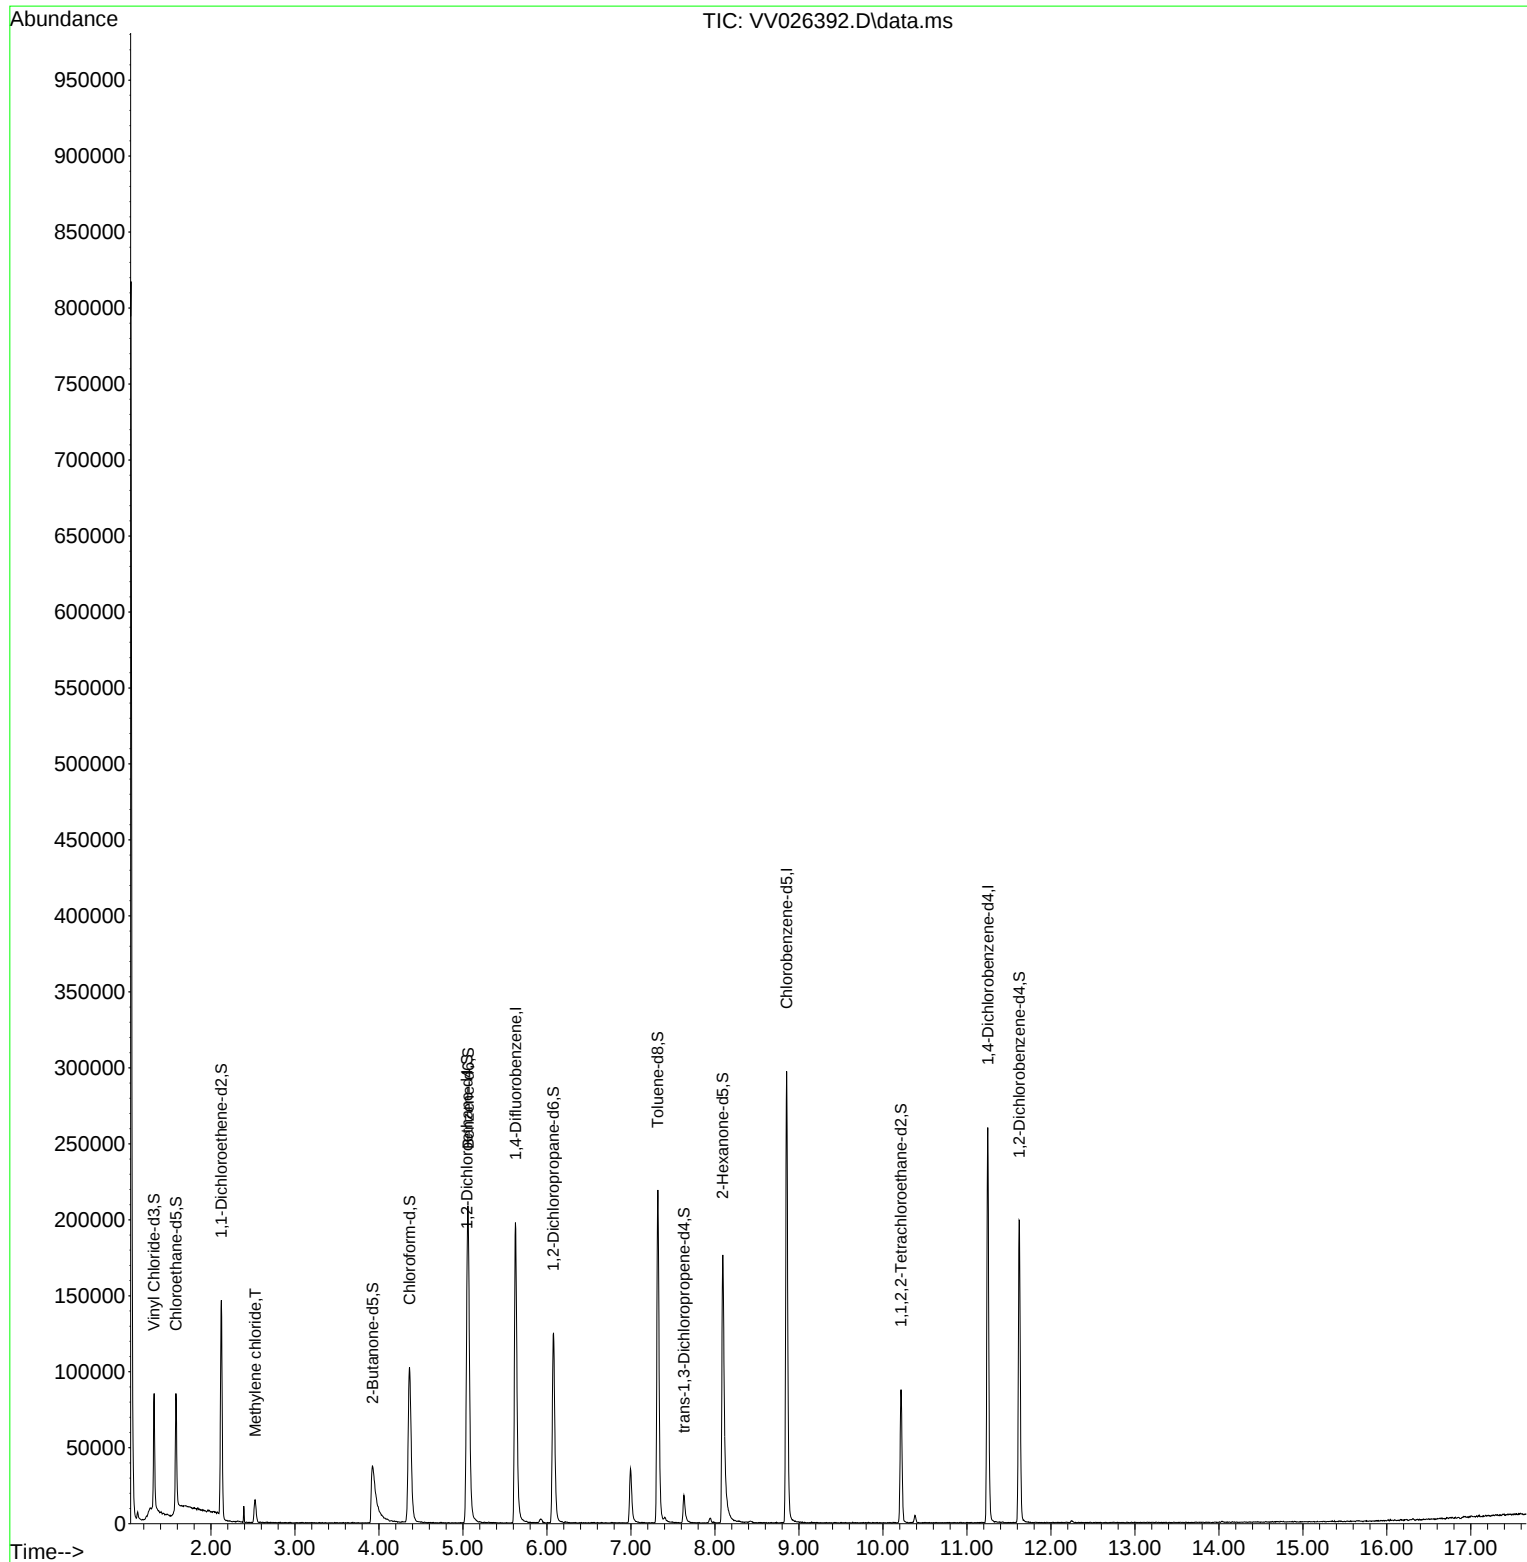

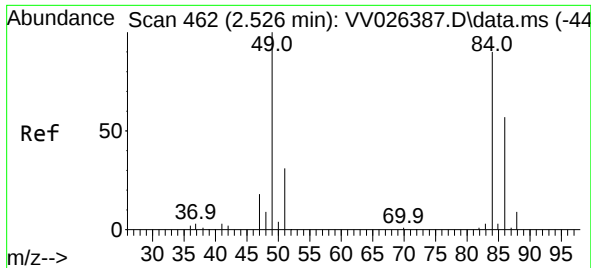

#16
Methylene chloride
Concen: 0.456 ug/L
RT: 2.526 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV026392.D
Acq: 17 Jun 2022 20:04

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

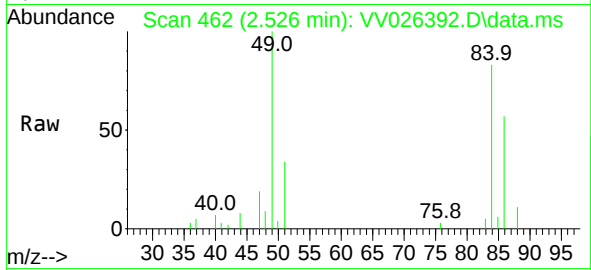

Tgt Ion: 84 Resp: 6545
Ion Ratio Lower Upper
84 100
86 68.9 44.0 81.8
49 120.5 77.3 143.7

