

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061722\
 Data File : VW026400.D
 Acq On : 17 Jun 2022 23:16
 Operator : SY/MD
 Sample : N3278-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE9

Quant Time: Jun 18 01:19:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	189518	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	184154	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	74099	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	47853	2.907	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	58.200%	
7) Chloroethane-d5	1.584	69	46336	3.580	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.600%	
11) 1,1-Dichloroethene-d2	2.124	63	70749	2.503	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	50.000%#	
20) 2-Butanone-d5	3.924	46	89523	55.736	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	111.480%	
24) Chloroform-d	4.362	84	109416	4.535	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
26) 1,2-Dichloroethane-d4	5.047	65	46525	4.558	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.200%	
32) Benzene-d6	5.063	84	193174	3.924	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.400%	
36) 1,2-Dichloropropane-d6	6.079	67	62317	4.337	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.800%	
41) Toluene-d8	7.320	98	146641	3.266	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	65.400%#	
43) trans-1,3-Dichloroprop...	7.632	79	11373	2.441	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	48.800%#	
46) 2-Hexanone-d5	8.091	63	58222	41.366	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.740%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43634	4.929	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	52813	4.627	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.600%	
Target Compounds					Qvalue	
13) Acetone	2.214	43	20686	16.618	ug/L	94
34) Trichloroethene	5.924	95	13613	1.056	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026400.D
Acq On : 17 Jun 2022 23:16
Operator : SY/MD
Sample : N3278-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE9

Quant Time: Jun 18 01:19:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 18 01:02:22 2022
Response via : Initial Calibration

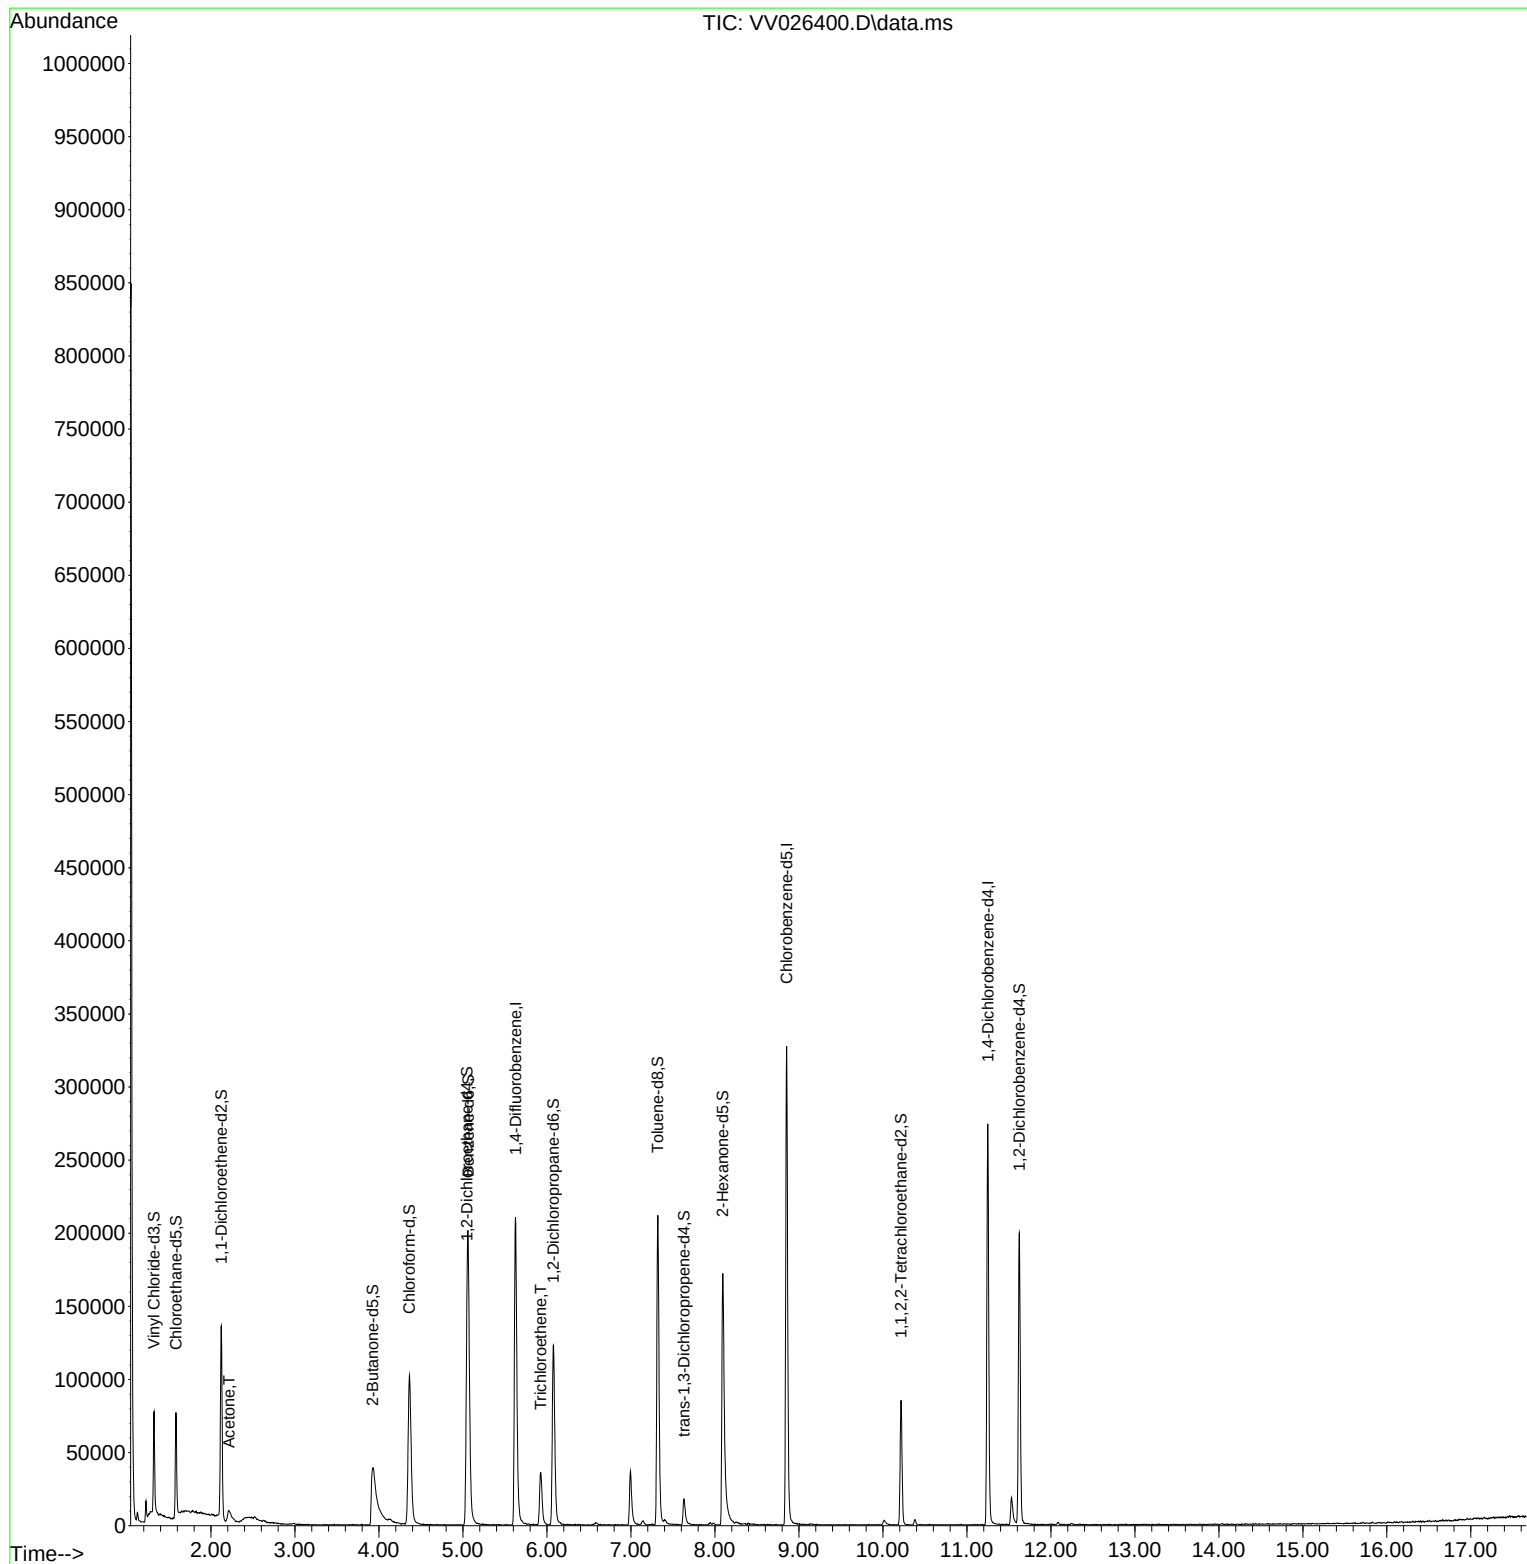

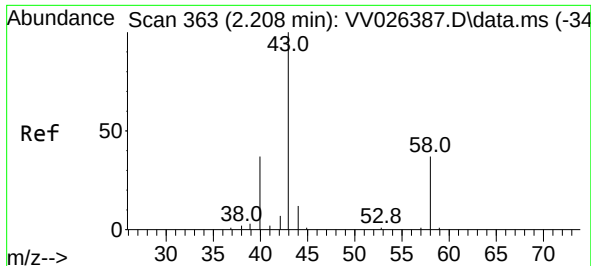

#13

Acetone

Concen: 16.618 ug/L

RT: 2.214 min Scan# 30

Delta R.T. 0.006 min

Lab File: VV026400.D

Acq: 17 Jun 2022 23:16

Instrument :

MSVOA_V

ClientSampleId :





C0BE9

Tgt Ion: 43 Resp: 20686

Ion Ratio Lower Upper

43 100

58 26.7 0.0 60.0

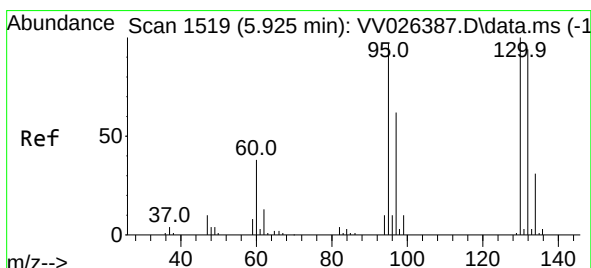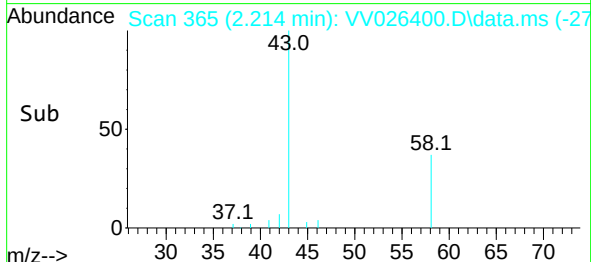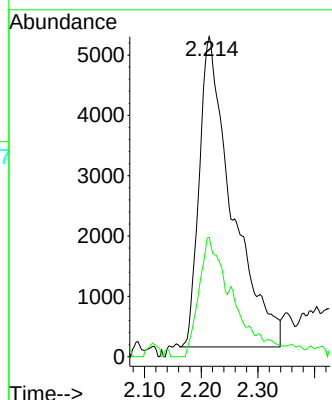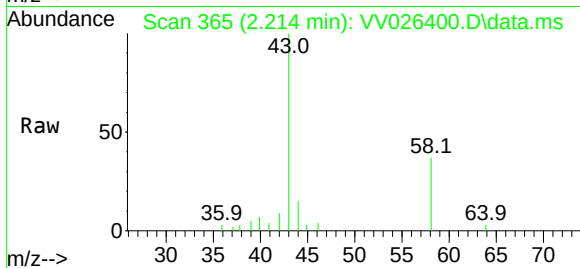

#34

Trichloroethene

Concen: 1.056 ug/L

RT: 5.924 min Scan# 1519

Delta R.T. -0.000 min

Lab File: VV026400.D

Acq: 17 Jun 2022 23:16

Tgt Ion: 95 Resp: 13613

Ion Ratio Lower Upper

95 100

97 64.5 46.5 86.3

132 95.7 68.8 127.8

130 100.2 73.6 136.6

