

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW061722\  
 Data File : VW026404.D  
 Acq On : 18 Jun 2022 00:52  
 Operator : SY/MD  
 Sample : N3358-03  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 36 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW4R9

Quant Time: Jun 18 01:20:09 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR061522WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 18 01:02:22 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon           | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|----------------|----------|--------|----------|----------|
| -----                         |        |                |          |        |          |          |
| Internal Standards            |        |                |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.625  | 114            | 175118   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.853  | 117            | 172058   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152            | 67797    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |        |                |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.323  | 65             | 48753    | 3.205  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =      | 64.200%  |          |
| 7) Chloroethane-d5            | 1.584  | 69             | 47112    | 3.939  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =      | 78.800%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.124  | 63             | 71509    | 2.738  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =      | 54.800%# |          |
| 20) 2-Butanone-d5             | 3.931  | 46             | 73775    | 49.708 | ug/L     | 0.01     |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =      | 99.420%  |          |
| 24) Chloroform-d              | 4.365  | 84             | 111923   | 5.020  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 100.400% |          |
| 26) 1,2-Dichloroethane-d4     | 5.047  | 65             | 45135    | 4.785  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 95.800%  |          |
| 32) Benzene-d6                | 5.063  | 84             | 192910   | 4.194  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =      | 83.800%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.075  | 67             | 64562    | 4.809  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =      | 96.200%  |          |
| 41) Toluene-d8                | 7.320  | 98             | 146333   | 3.489  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =      | 69.800%# |          |
| 43) trans-1,3-Dichloroprop... | 7.632  | 79             | 12322    | 2.830  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =      | 56.600%  |          |
| 46) 2-Hexanone-d5             | 8.091  | 63             | 63024    | 47.925 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =      | 95.860%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84             | 44539    | 5.385  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =      | 107.800% |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152            | 52199    | 4.998  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =      | 100.000% |          |
| Target Compounds              |        |                |          |        |          |          |
|                               |        |                |          |        | Qvalue   |          |
| 14) Carbon disulfide          | 2.310  | 76             | 44909    | 1.646  | ug/L     | 100      |
| -----                         |        |                |          |        |          |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061722\  
Data File : VV026404.D  
Acq On : 18 Jun 2022 00:52  
Operator : SY/MD  
Sample : N3358-03  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW4R9

Quant Time: Jun 18 01:20:09 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR061522WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 18 01:02:22 2022  
Response via : Initial Calibration

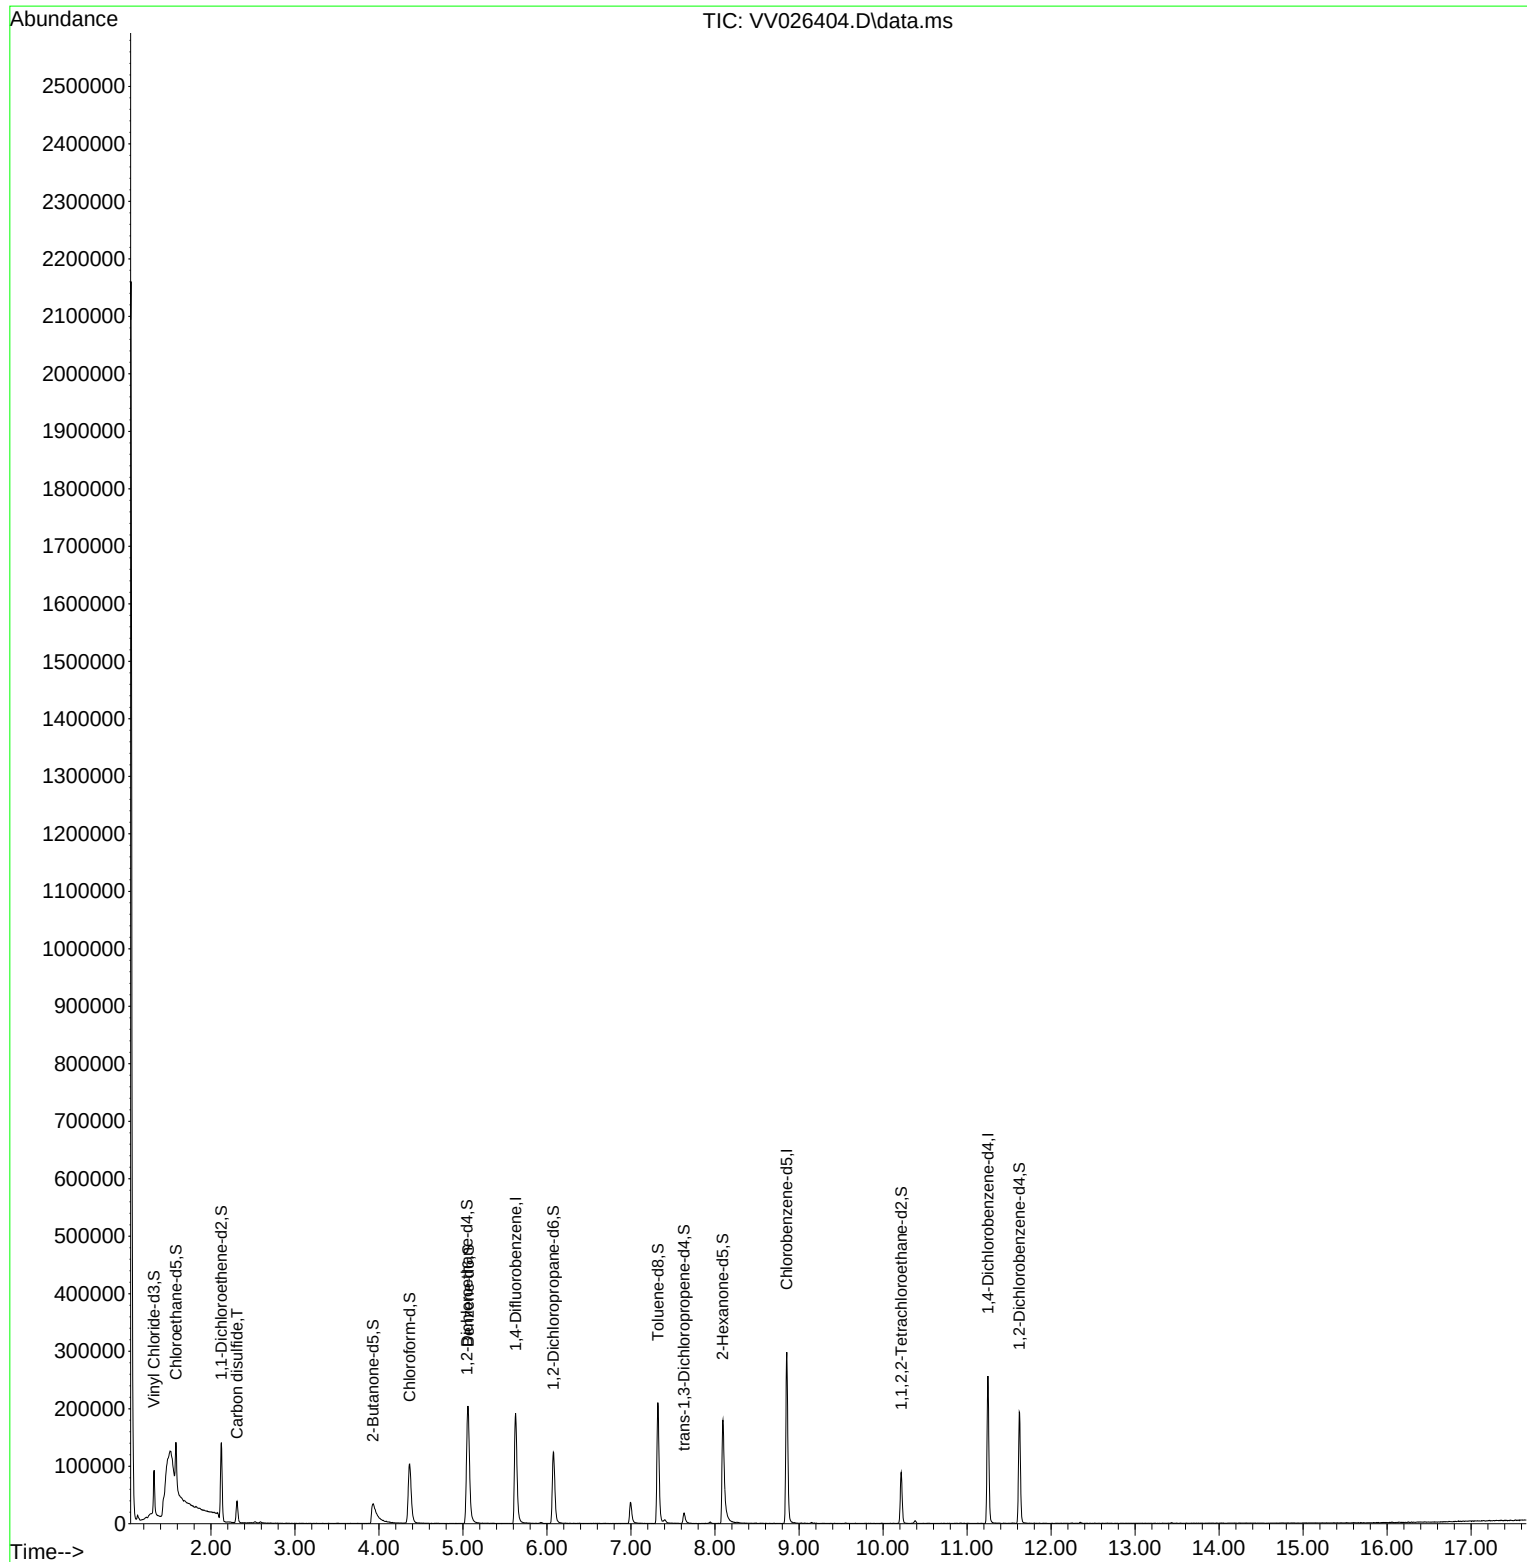

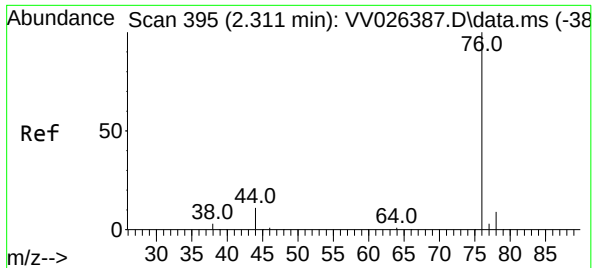

#14  
Carbon disulfide  
Concen: 1.646 ug/L  
RT: 2.310 min Scan# 395  
Delta R.T. -0.000 min  
Lab File: VV026404.D  
Acq: 18 Jun 2022 00:52

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW4R9

Tgt Ion: 76 Resp: 44909  
Ion Ratio Lower Upper  
76 100  
78 9.5 7.7 11.5

