

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061722\
 Data File : VW026405.D
 Acq On : 18 Jun 2022 01:16
 Operator : SY/MD
 Sample : N3358-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4S0

Quant Time: Jun 18 02:13:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 01:02:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	186927	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	178512	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70938	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.323	65	45357	2.794	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.800%
7) Chloroethane-d5	1.584	69	43416	3.401	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.000%
11) 1,1-Dichloroethene-d2	2.124	63	65569	2.352	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	47.000%#
20) 2-Butanone-d5	3.931	46	79626	50.261	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.520%
24) Chloroform-d	4.365	84	103130	4.334	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
26) 1,2-Dichloroethane-d4	5.047	65	42928	4.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.063	84	177201	3.713	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.200%
36) 1,2-Dichloropropane-d6	6.079	67	58353	4.189	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.800%
41) Toluene-d8	7.320	98	135472	3.113	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	62.200%#
43) trans-1,3-Dichloroprop...	7.632	79	10965	2.428	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	48.600%#
46) 2-Hexanone-d5	8.092	63	57273	41.978	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39885	4.648	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	49308	4.513	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.200%
Target Compounds						Qvalue
14) Carbon disulfide	2.311	76	45542	1.564	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026405.D
Acq On : 18 Jun 2022 01:16
Operator : SY/MD
Sample : N3358-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4S0

Quant Time: Jun 18 02:13:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 18 01:02:22 2022
Response via : Initial Calibration

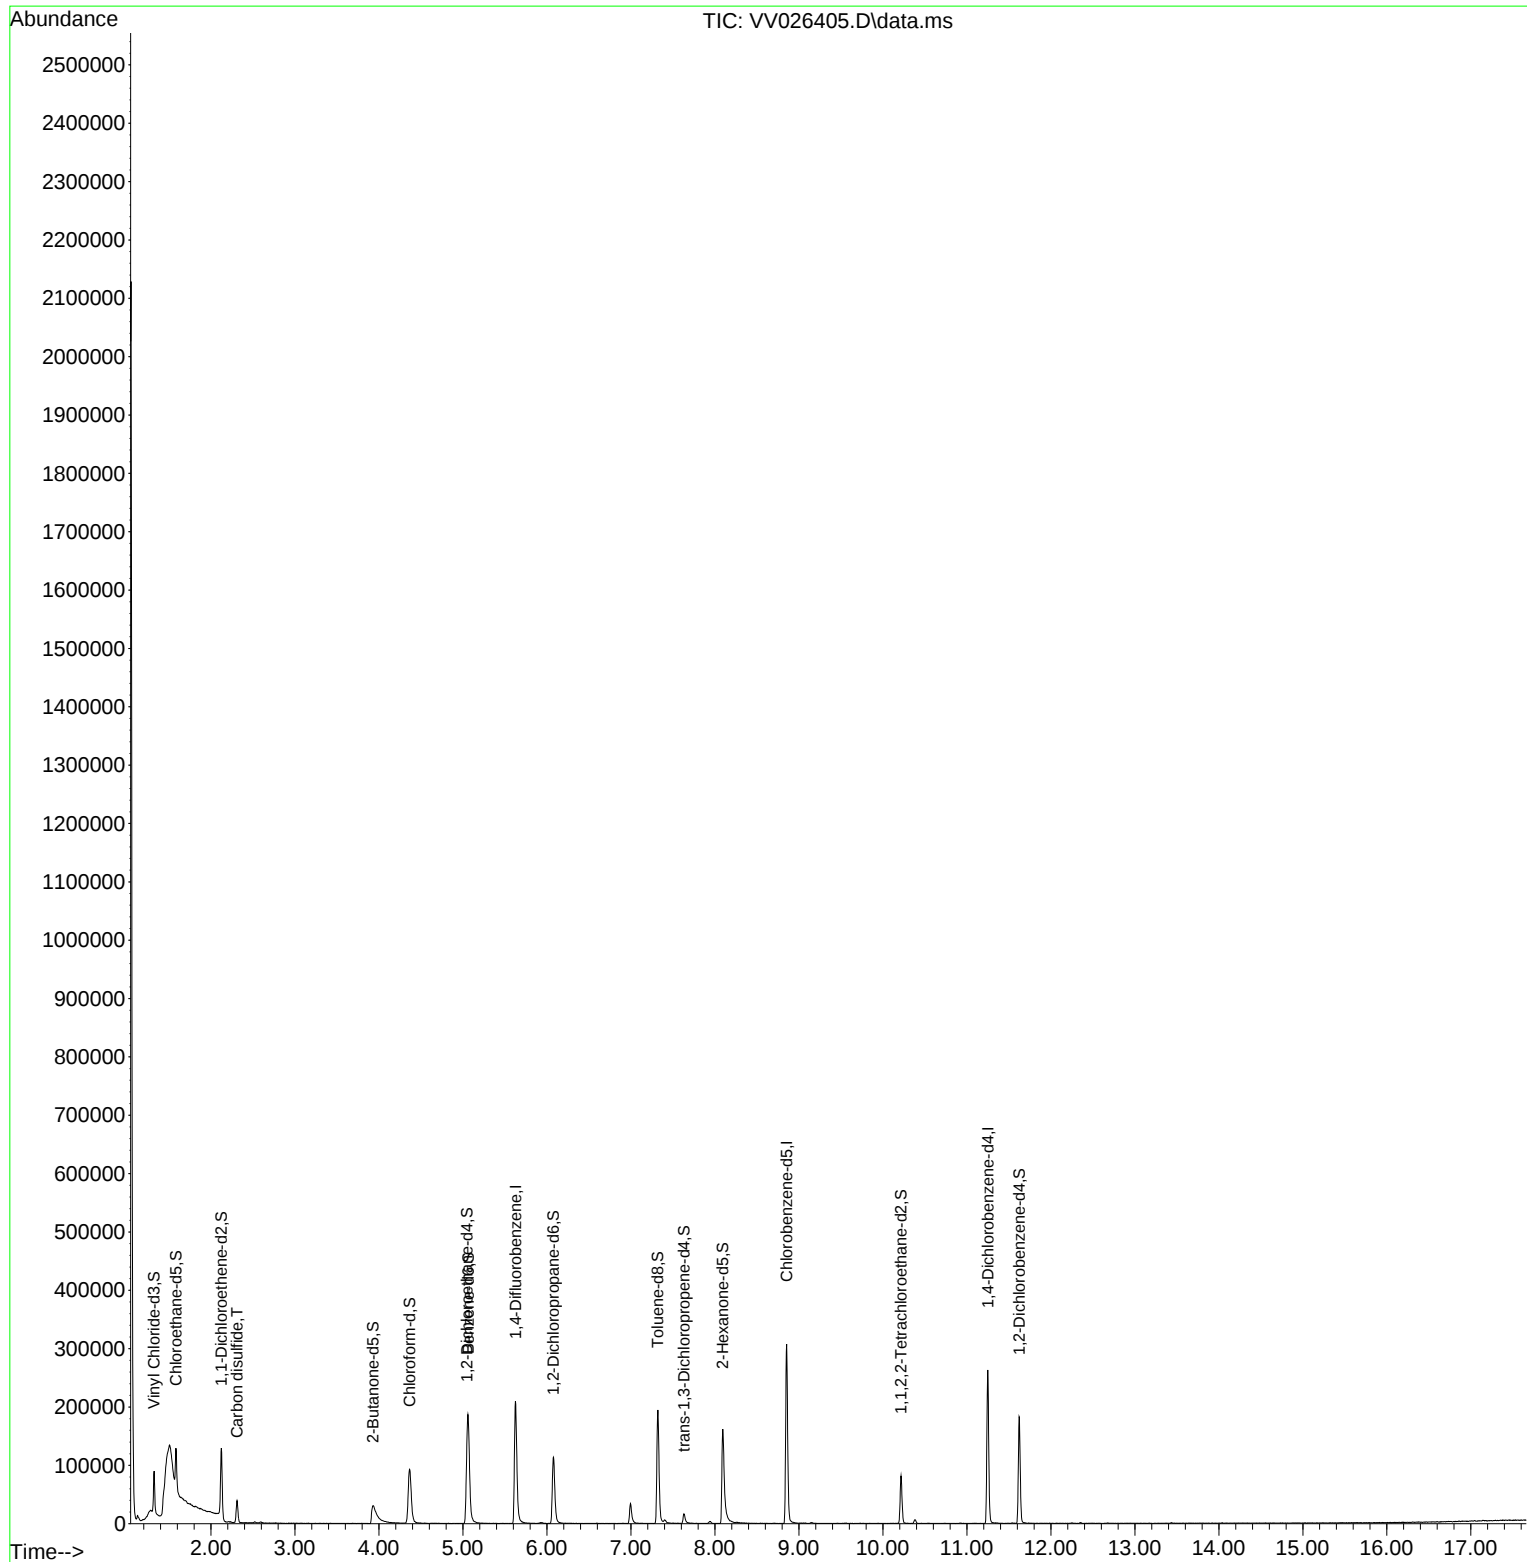

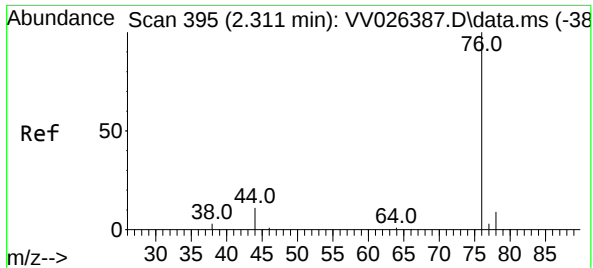

#14
Carbon disulfide
Concen: 1.564 ug/L
RT: 2.311 min Scan# 395
Delta R.T. -0.000 min
Lab File: VV026405.D
Acq: 18 Jun 2022 01:16

Instrument :
MSVOA_V
ClientSampleId :
EW4S0

Tgt Ion: 76 Resp: 45542
Ion Ratio Lower Upper
76 100
78 8.8 7.7 11.5

