

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026373.D
 Acq On : 17 Jun 2022 11:51
 Operator : SY/MD
 Sample : N3318-18DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ72DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	52	63	64	rBV2	11063	15516	2.75%	0.293%
2	1.320	81	87	98	rVB	86571	91154	16.18%	1.723%
3	1.552	144	159	160	rBV2	10422	20844	3.70%	0.394%
4	1.581	162	168	187	rVB	88656	114013	20.23%	2.155%
5	2.124	326	337	358	rVB3	249623	428421	76.03%	8.099%
6	2.520	450	460	477	rBV	30814	52485	9.31%	0.992%
7	3.201	654	672	694	rBV	143374	305833	54.27%	5.782%
8	3.918	882	895	932	rBV3	56262	216419	38.41%	4.091%
9	4.359	1015	1032	1054	rBV	107680	270444	47.99%	5.113%
10	5.053	1232	1248	1277	rBV2	225036	563508	100.00%	10.653%
11	5.622	1412	1425	1451	rBV2	209754	431775	76.62%	8.162%
12	5.921	1505	1518	1538	rBV	84478	171444	30.42%	3.241%
13	6.072	1553	1565	1593	rBV	133437	277610	49.26%	5.248%
14	6.992	1841	1851	1873	rBV2	39356	74856	13.28%	1.415%
15	7.317	1939	1952	1972	rBV	246147	439006	77.91%	8.299%
16	7.629	2039	2049	2066	rBV2	19851	37726	6.69%	0.713%
17	8.092	2181	2193	2230	rBV2	164466	357849	63.50%	6.765%
18	8.854	2416	2430	2453	rBV	316536	529798	94.02%	10.015%
19	10.217	2842	2854	2874	rBV	85299	138106	24.51%	2.611%
20	11.246	3163	3174	3194	rBV	273648	419426	74.43%	7.929%
21	11.622	3279	3291	3309	rBV	210816	333615	59.20%	6.307%




Sum of corrected areas: 5289848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026373.D
Acq On : 17 Jun 2022 11:51
Operator : SY/MD
Sample : N3318-18DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ72DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

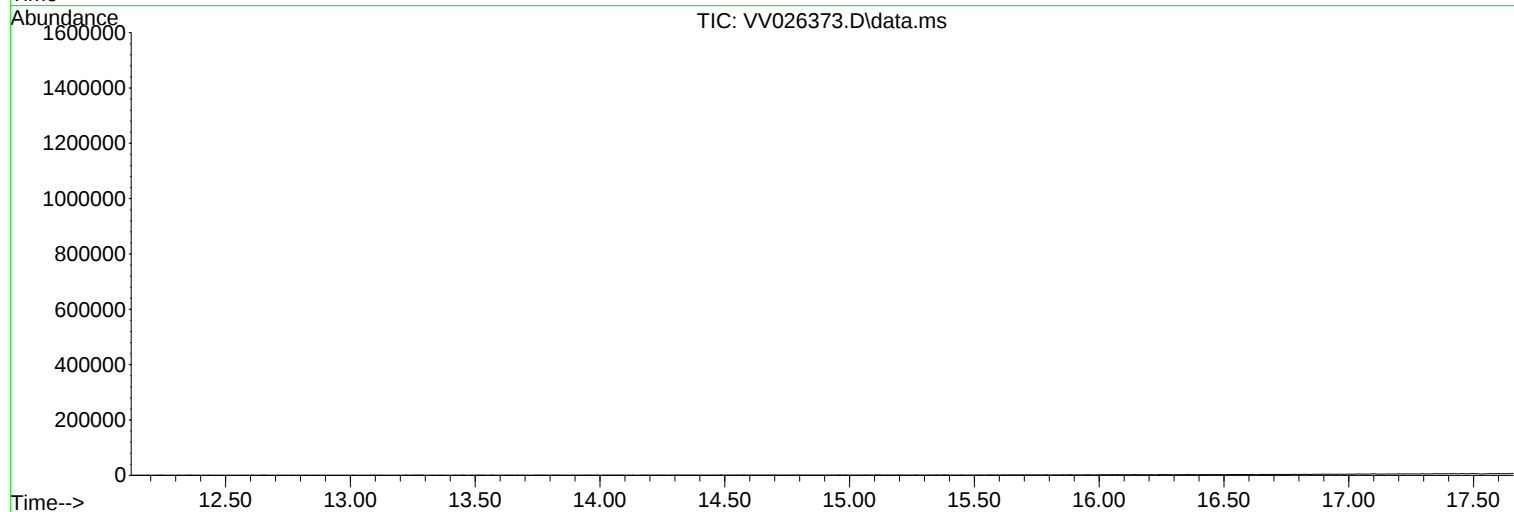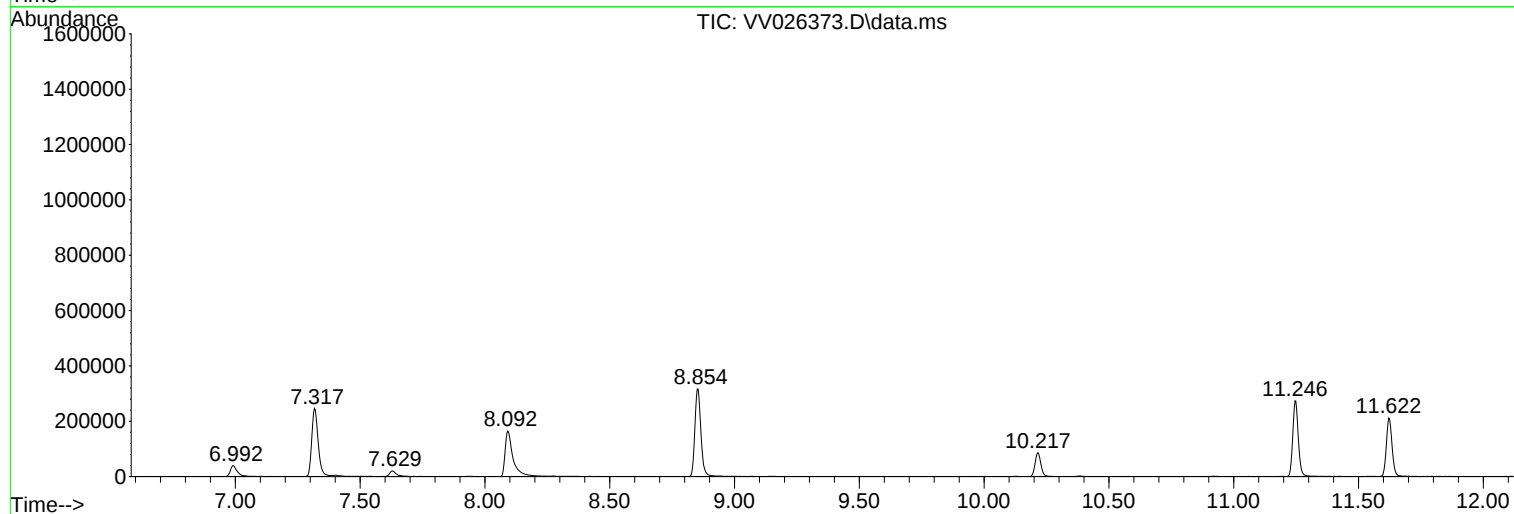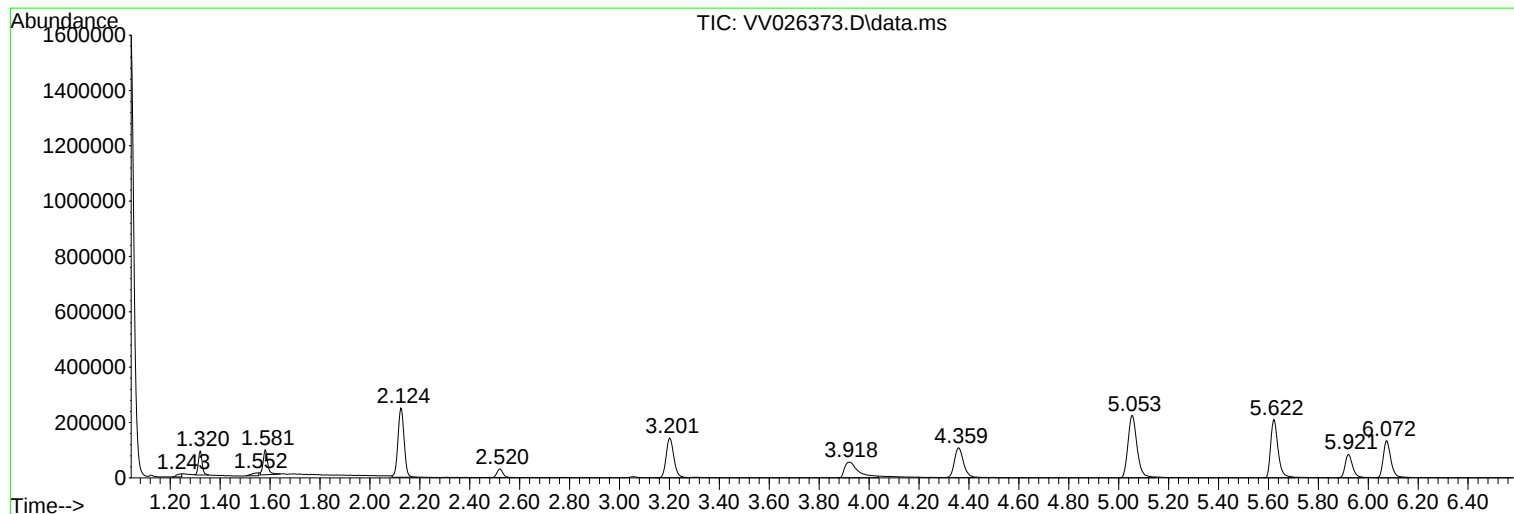

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026373.D
Acq On : 17 Jun 2022 11:51
Operator : SY/MD
Sample : N3318-18DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ72DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026373.D
Acq On : 17 Jun 2022 11:51
Operator : SY/MD
Sample : N3318-18DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ72DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc