

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026375.D
 Acq On : 17 Jun 2022 12:39
 Operator : SY/MD
 Sample : N3318-02DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ56DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.249	54	65	67	rBV	15392	23231	4.33%	0.469%
2	1.323	81	88	104	rVB2	95269	109635	20.41%	2.213%
3	1.552	142	159	160	rBV2	23096	48737	9.08%	0.984%
4	1.584	162	169	182	rVB	85196	119839	22.32%	2.419%
5	2.124	327	337	354	rVB2	167516	266287	49.58%	5.375%
6	2.523	451	461	480	rVB	18064	31340	5.84%	0.633%
7	3.928	883	898	940	rBV4	140954	439435	81.83%	8.869%
8	4.362	1018	1033	1057	rBV	102050	254634	47.42%	5.139%
9	5.059	1234	1250	1275	rBV2	217819	537032	100.00%	10.839%
10	5.625	1414	1426	1445	rBV2	213268	430568	80.18%	8.690%
11	5.924	1508	1519	1542	rBV	74554	152957	28.48%	3.087%
12	6.079	1553	1567	1598	rVB	125820	265141	49.37%	5.351%
13	6.995	1842	1852	1868	rBV2	36571	70240	13.08%	1.418%
14	7.320	1942	1953	1972	rBV	234564	414929	77.26%	8.375%
15	7.632	2039	2050	2066	rBV	19449	35451	6.60%	0.716%
16	8.095	2182	2194	2229	rBV2	170283	354789	66.06%	7.161%
17	8.854	2419	2430	2456	rBV	315519	522555	97.30%	10.547%
18	10.217	2842	2854	2868	rBV2	84212	134667	25.08%	2.718%
19	11.249	3161	3175	3195	rBV	271958	423417	78.84%	8.546%
20	11.622	3277	3291	3312	rBV	202546	319685	59.53%	6.452%




Sum of corrected areas: 4954569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026375.D
Acq On : 17 Jun 2022 12:39
Operator : SY/MD
Sample : N3318-02DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ56DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

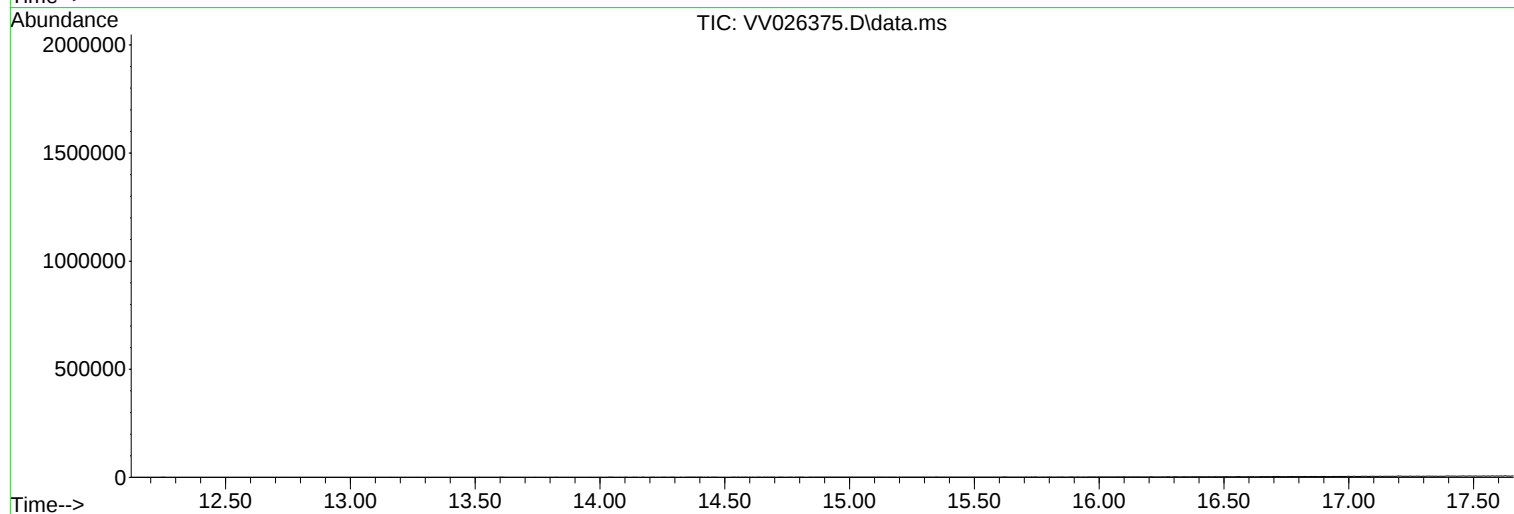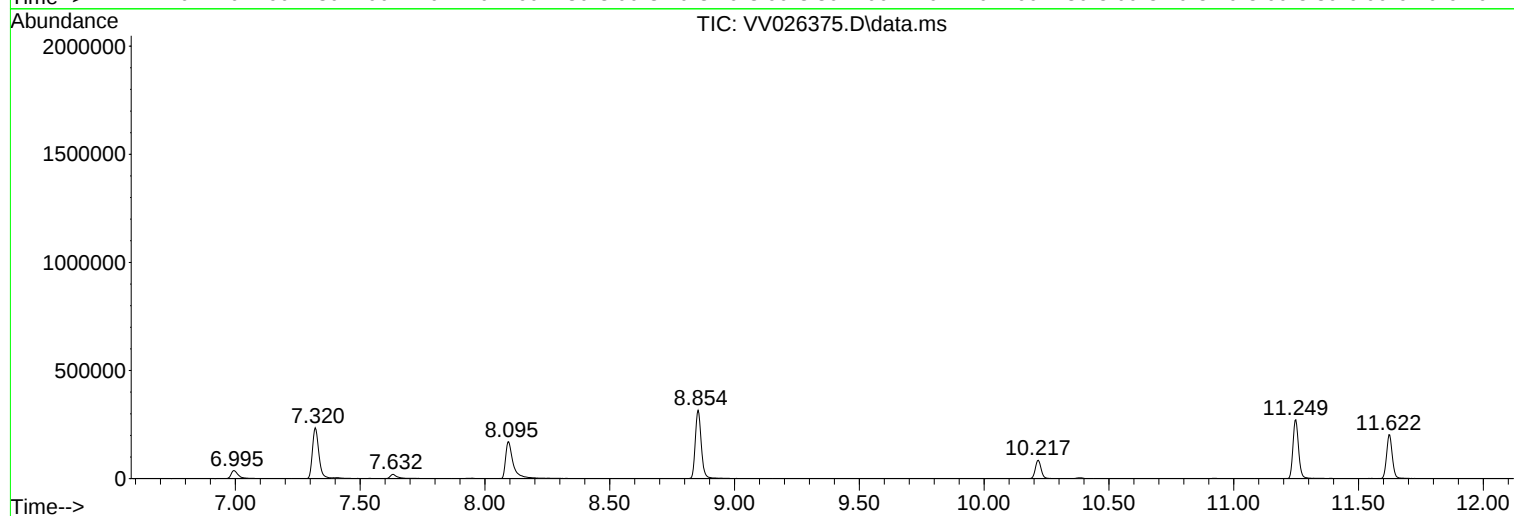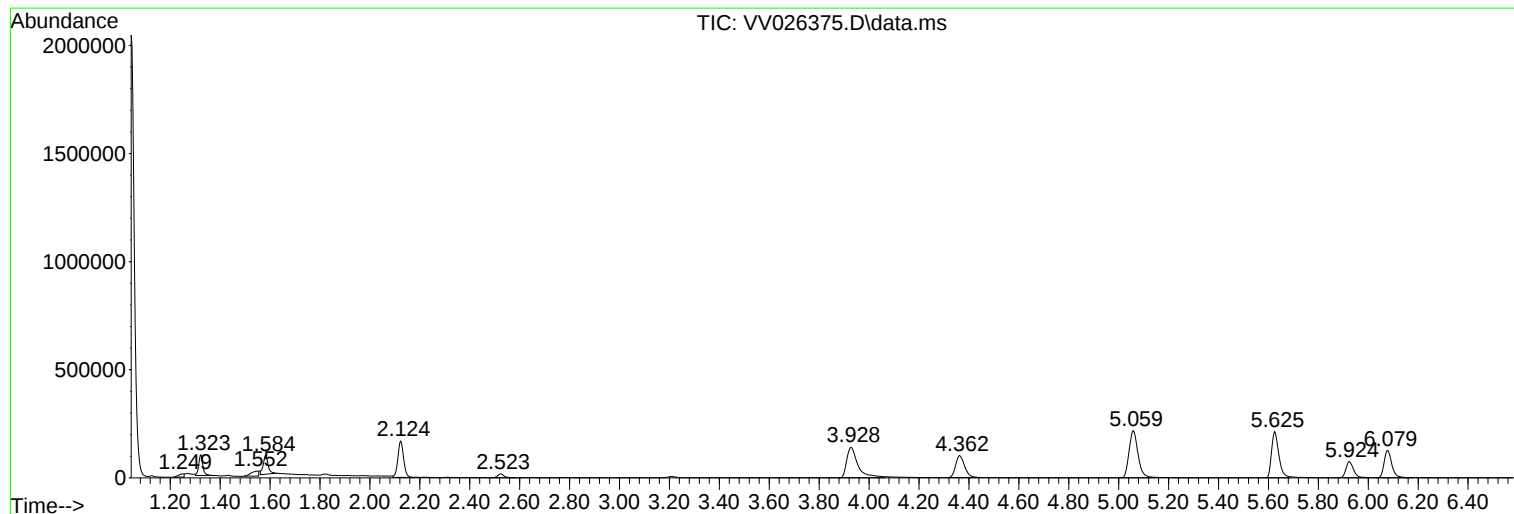

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026375.D
Acq On : 17 Jun 2022 12:39
Operator : SY/MD
Sample : N3318-02DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ56DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026375.D
Acq On : 17 Jun 2022 12:39
Operator : SY/MD
Sample : N3318-02DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ56DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc