

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026389.D
 Acq On : 17 Jun 2022 18:51
 Operator : SY/MD
 Sample : N3318-10 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ64

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	108	rBV2	147962	172561	34.71%	3.426%
2	1.584	141	169	187	rBV3	104876	297744	59.89%	5.912%
3	2.121	327	336	351	rVB	152456	231179	46.50%	4.590%
4	2.224	357	368	383	rVB2	17606	32506	6.54%	0.645%
5	2.523	452	461	473	rVB2	13772	23413	4.71%	0.465%
6	3.208	660	674	696	rBV	151356	316886	63.74%	6.292%
7	3.931	883	899	932	rBV2	156698	474590	95.46%	9.423%
8	4.365	1017	1034	1057	rBV	95557	239450	48.16%	4.754%
9	5.060	1235	1250	1276	rBV3	201140	497174	100.00%	9.872%
10	5.625	1412	1426	1454	rBV	196906	406598	81.78%	8.073%
11	6.079	1554	1567	1589	rBV2	118861	244517	49.18%	4.855%
12	6.995	1842	1852	1875	rBV2	34180	66934	13.46%	1.329%
13	7.320	1942	1953	1973	rBV	212228	374179	75.26%	7.430%
14	7.632	2041	2050	2070	rBV2	16444	32084	6.45%	0.637%
15	8.095	2183	2194	2224	rBV2	152815	319662	64.30%	6.347%
16	8.854	2419	2430	2453	rBV	298363	483468	97.24%	9.600%
17	10.217	2842	2854	2871	rBV	82099	126784	25.50%	2.517%
18	11.249	3164	3175	3197	rBV	259665	401259	80.71%	7.967%
19	11.622	3281	3291	3314	rBV	185059	295355	59.41%	5.864%




Sum of corrected areas: 5036343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026389.D
Acq On : 17 Jun 2022 18:51
Operator : SY/MD
Sample : N3318-10 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

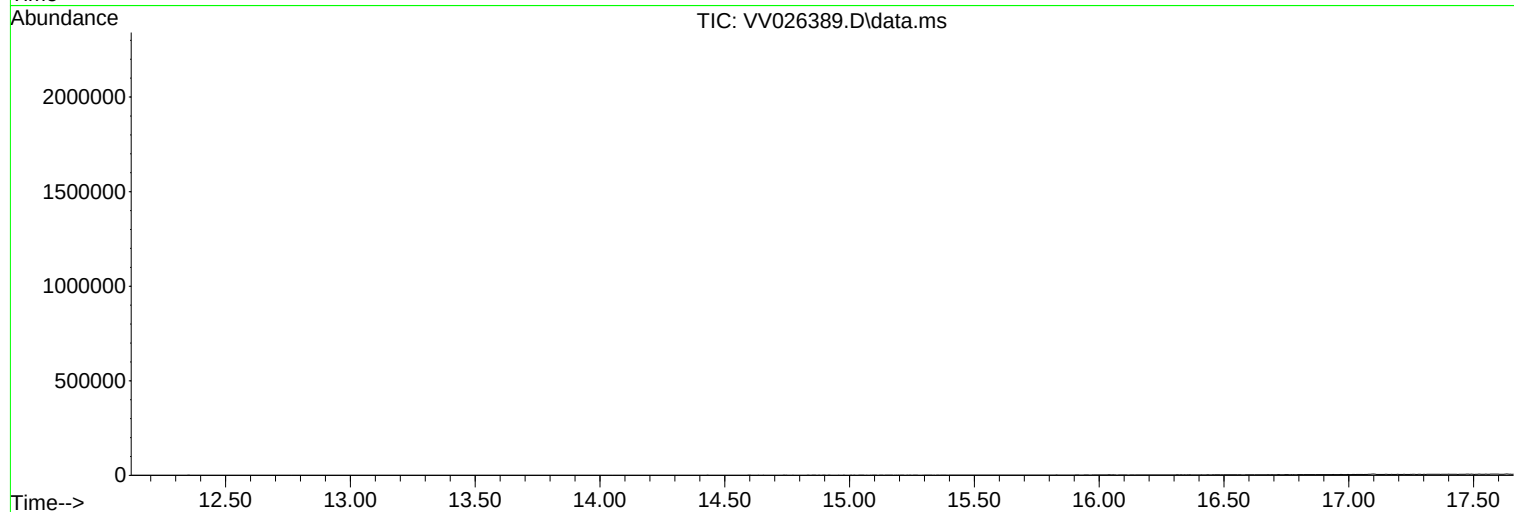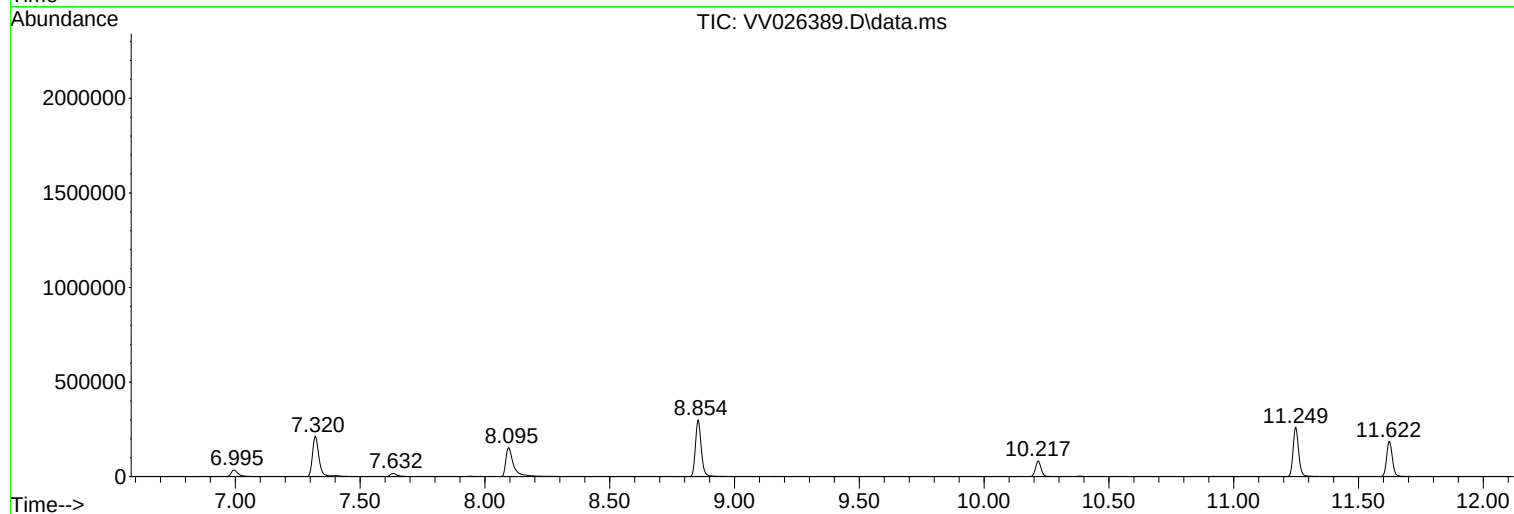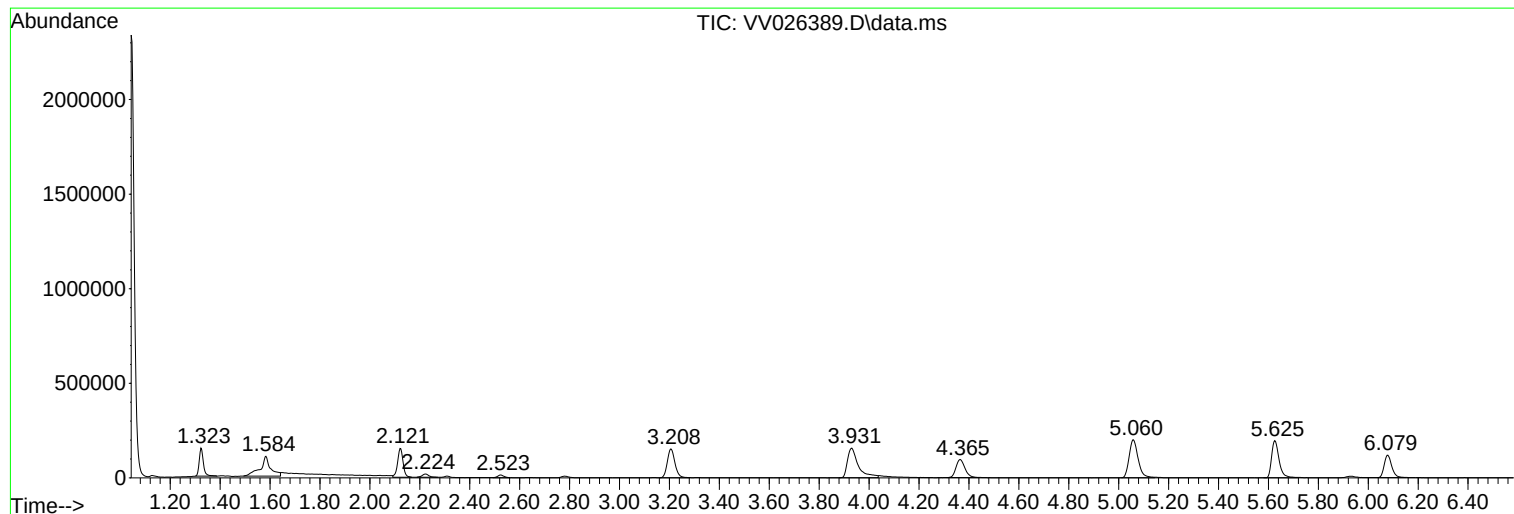

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026389.D
Acq On : 17 Jun 2022 18:51
Operator : SY/MD
Sample : N3318-10 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026389.D
Acq On : 17 Jun 2022 18:51
Operator : SY/MD
Sample : N3318-10 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc