

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026394.D
 Acq On : 17 Jun 2022 20:52
 Operator : SY/MD
 Sample : N3275-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	37	rVB4	7445	8927	1.84%	0.224%
2	1.282	63	75	79	rBV4	4535	10268	2.12%	0.258%
3	1.320	81	87	104	rVB	69104	78349	16.16%	1.965%
4	1.584	161	169	181	rBV	69692	87821	18.11%	2.202%
5	2.121	326	336	353	rVB	125248	186494	38.46%	4.677%
6	2.214	353	365	384	rVB2	5680	16722	3.45%	0.419%
7	3.925	887	897	935	rBV2	34007	144024	29.70%	3.612%
8	4.362	1018	1033	1056	rBV	93892	232245	47.89%	5.824%
9	5.060	1235	1250	1274	rBV3	184051	457302	94.30%	11.469%
10	5.625	1414	1426	1456	rBV	192780	397997	82.07%	9.981%
11	5.928	1505	1520	1533	rBV9	6790	15395	3.17%	0.386%
12	6.076	1554	1566	1589	rBV	114600	236889	48.85%	5.941%
13	6.995	1838	1852	1868	rBV2	31065	60676	12.51%	1.522%
14	7.320	1942	1953	1971	rBV	191252	339359	69.98%	8.511%
15	7.632	2042	2050	2075	rVB2	14962	29350	6.05%	0.736%
16	7.979	2151	2158	2173	rVB3	10513	18892	3.90%	0.474%
17	8.095	2184	2194	2227	rBV2	160412	335249	69.13%	8.408%
18	8.854	2419	2430	2456	rBV	293611	484938	100.00%	12.162%
19	10.217	2842	2854	2873	rBV2	81287	128901	26.58%	3.233%
20	10.381	2893	2905	2915	rBV2	7129	11053	2.28%	0.277%
21	11.249	3164	3175	3193	rBV	255410	398686	82.21%	9.999%
22	11.532	3254	3263	3275	rBV4	11227	21891	4.51%	0.549%
23	11.622	3282	3291	3309	rVB	185921	285994	58.98%	7.172%




Sum of corrected areas: 3987422

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026394.D
Acq On : 17 Jun 2022 20:52
Operator : SY/MD
Sample : N3275-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

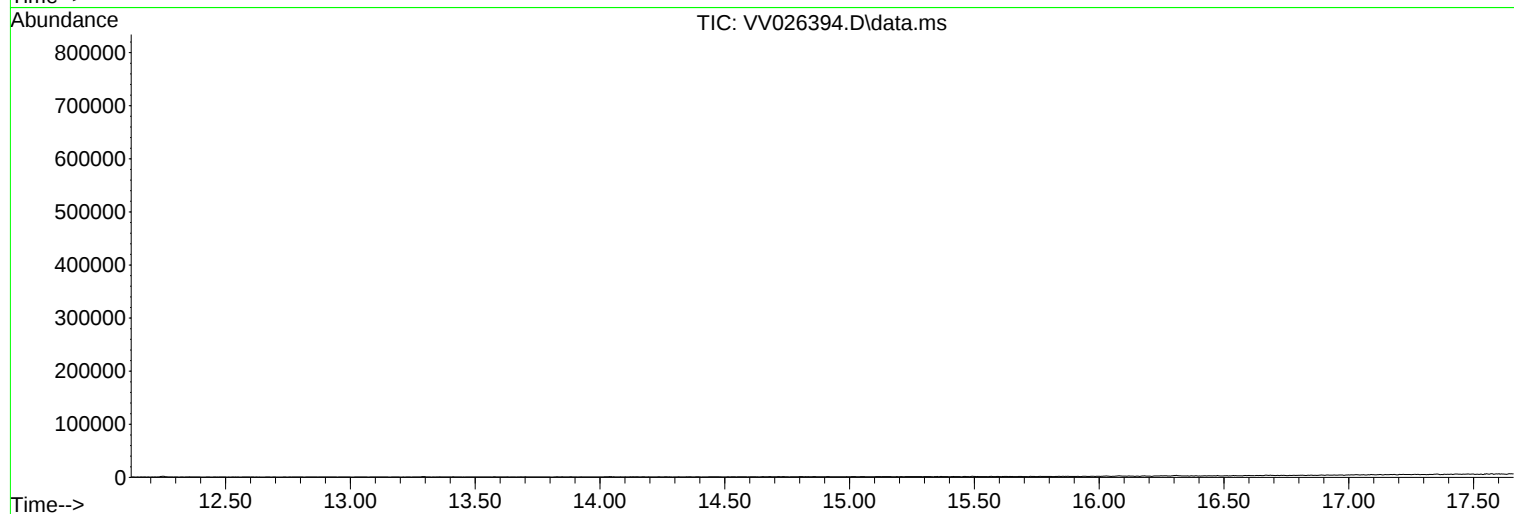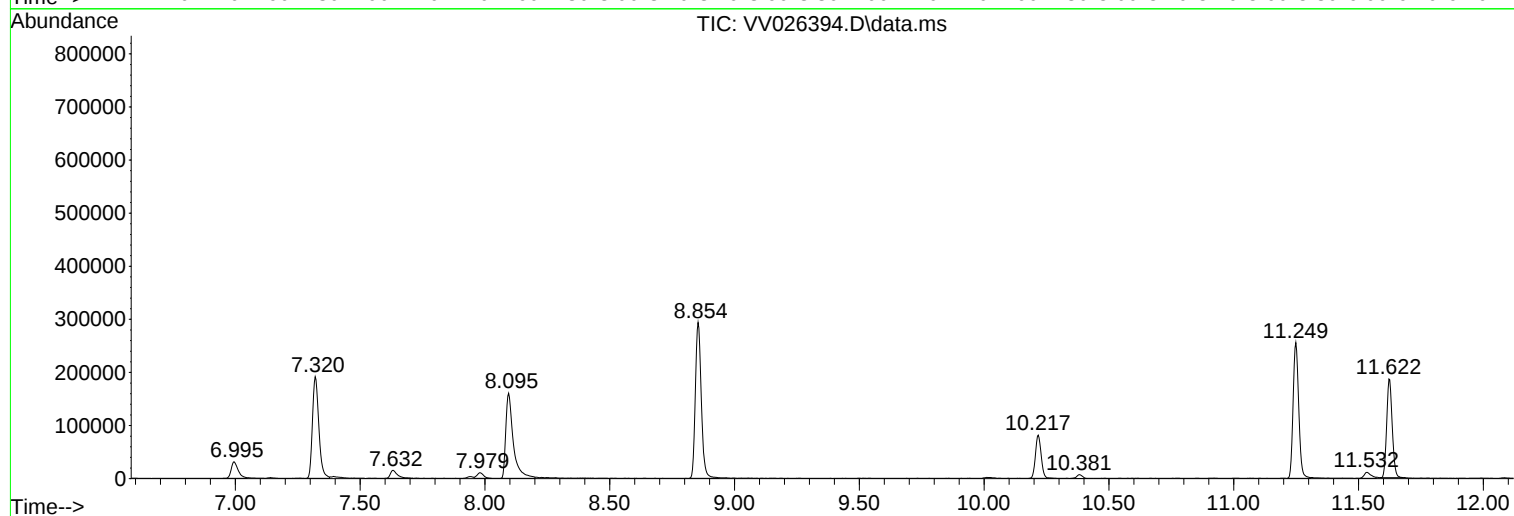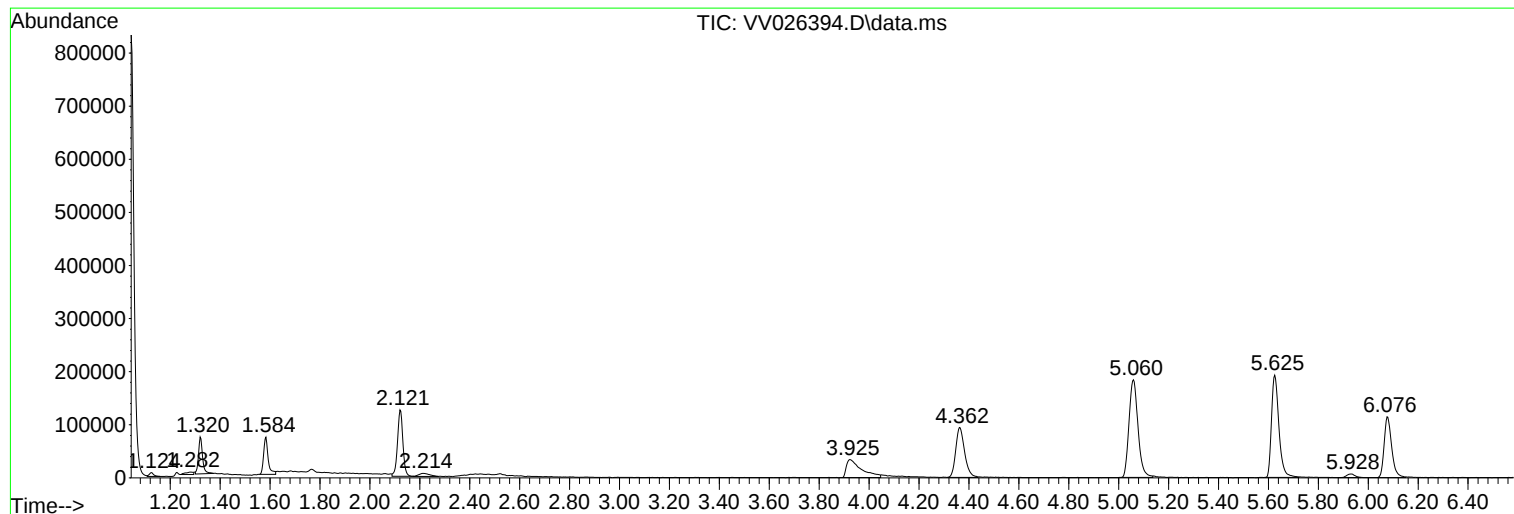

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026394.D
Acq On : 17 Jun 2022 20:52
Operator : SY/MD
Sample : N3275-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026394.D
Acq On : 17 Jun 2022 20:52
Operator : SY/MD
Sample : N3275-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------