

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026395.D
 Acq On : 17 Jun 2022 21:16
 Operator : SY/MD
 Sample : N3275-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	22	27	34	rVB3	7147	7080	1.45%	0.157%
2	1.227	52	58	62	rBV	5560	6057	1.24%	0.134%
3	1.323	81	88	102	rVB	68328	75646	15.50%	1.675%
4	1.584	161	169	180	rBV	69173	85110	17.43%	1.884%
5	1.770	219	227	236	rVB	21601	29205	5.98%	0.646%
6	2.124	327	337	351	rVB	130783	191975	39.33%	4.250%
7	2.211	352	364	389	rBV	19886	66695	13.66%	1.476%
8	2.407	399	425	426	rBV4	30560	85050	17.42%	1.883%
9	3.928	884	898	931	rBV2	37629	162620	33.31%	3.600%
10	4.365	1018	1034	1060	rBV	95461	245595	50.31%	5.437%
11	5.059	1235	1250	1283	rBV3	193950	482603	98.86%	10.683%
12	5.625	1413	1426	1459	rBV	197699	406730	83.32%	9.004%
13	5.924	1506	1519	1545	rBV2	98010	199460	40.86%	4.415%
14	6.079	1553	1567	1590	rBV	117130	244057	49.99%	5.403%
15	6.995	1840	1852	1873	rBV2	34438	66161	13.55%	1.465%
16	7.320	1939	1953	1973	rBV	204043	359917	73.73%	7.967%
17	7.397	1973	1977	1991	rVB4	3682	6872	1.41%	0.152%
18	7.632	2041	2050	2073	rBV3	16353	32321	6.62%	0.715%
19	7.979	2149	2158	2175	rVB3	26472	47012	9.63%	1.041%
20	8.095	2184	2194	2225	rBV2	167741	351729	72.05%	7.786%
21	8.853	2419	2430	2453	rBV	301525	488166	100.00%	10.806%
22	10.217	2842	2854	2870	rBV2	84107	133803	27.41%	2.962%
23	10.381	2896	2905	2915	rBV2	4643	6972	1.43%	0.154%
24	11.249	3162	3175	3190	rBV	257744	403544	82.67%	8.933%
25	11.532	3253	3263	3280	rBV4	13968	28870	5.91%	0.639%
26	11.625	3281	3292	3309	rVB	187777	304160	62.31%	6.733%




Sum of corrected areas: 4517410

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026395.D
Acq On : 17 Jun 2022 21:16
Operator : SY/MD
Sample : N3275-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

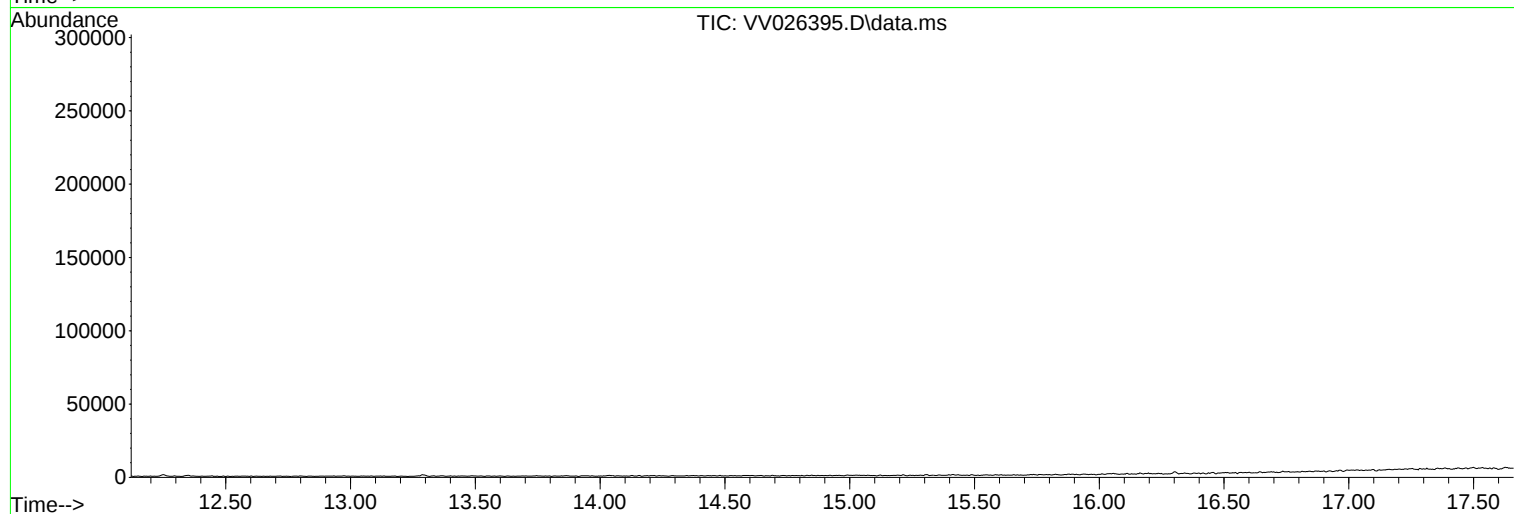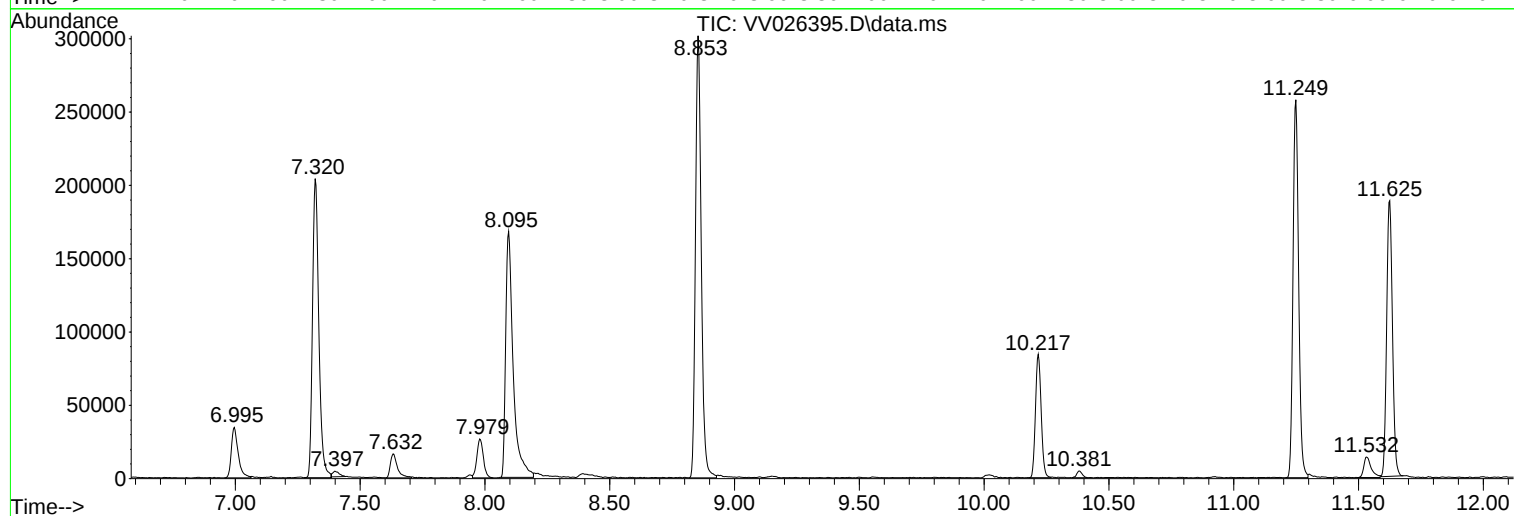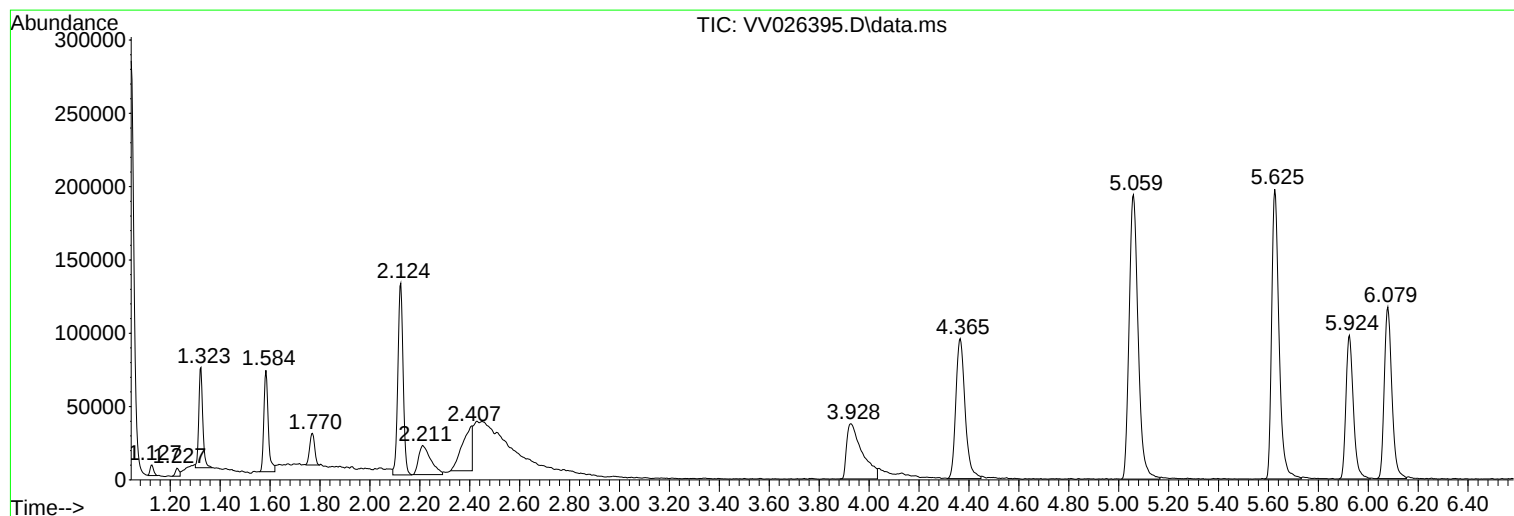

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026395.D
Acq On : 17 Jun 2022 21:16
Operator : SY/MD
Sample : N3275-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.407	1.05 ug/L	85050	1,4-Difluorobenzene	5.625

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

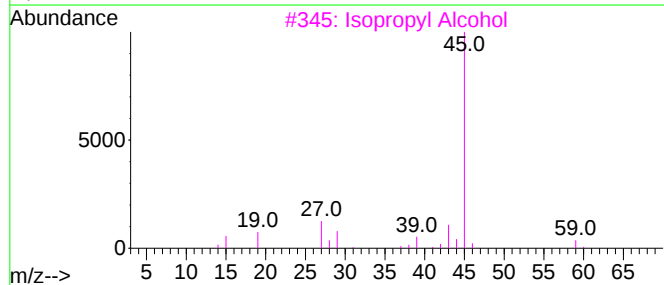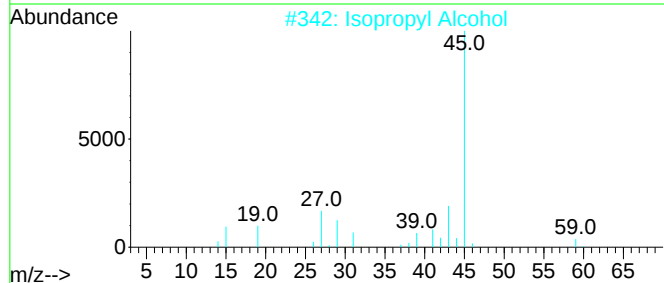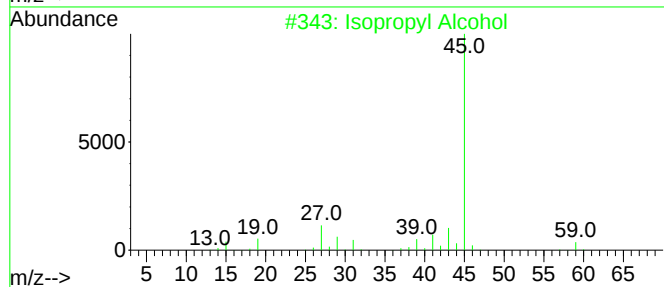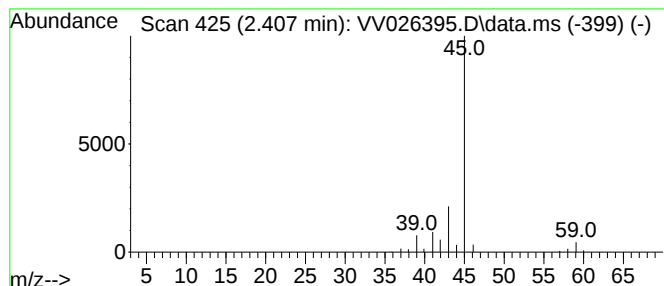

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026395.D
Acq On : 17 Jun 2022 21:16
Operator : SY/MD
Sample : N3275-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.407	1.1	ug/L	85050	1	5.625	406730	5.0