

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026401.D
 Acq On : 17 Jun 2022 23:40
 Operator : SY/MD
 Sample : N3278-10 10000X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	100	rVB	74364	80534	2.62%	1.077%
2	1.584	161	169	180	rBV	75559	90296	2.94%	1.207%
3	2.124	328	337	350	rVB	139950	199552	6.50%	2.668%
4	2.523	451	461	479	rVB	26209	44259	1.44%	0.592%
5	3.931	880	899	930	rBV3	48666	209891	6.83%	2.807%
6	4.365	1018	1034	1060	rBV2	102013	254943	8.30%	3.409%
7	5.060	1234	1250	1278	rBV2	205421	515141	16.77%	6.889%
8	5.626	1414	1426	1455	rBV	204773	419232	13.65%	5.606%
9	5.918	1503	1517	1548	rBV	1604065	3071373	100.00%	41.072%
10	6.076	1554	1566	1590	rVB	128419	264095	8.60%	3.532%
11	6.995	1841	1852	1872	rBV	38529	72918	2.37%	0.975%
12	7.320	1942	1953	1971	rBV	222439	391958	12.76%	5.241%
13	7.629	2040	2049	2069	rBV	19484	37866	1.23%	0.506%
14	7.979	2148	2158	2173	rVB	47122	81242	2.65%	1.086%
15	8.095	2184	2194	2235	rBV2	176828	373082	12.15%	4.989%
16	8.854	2419	2430	2453	rBV	312829	512246	16.68%	6.850%
17	10.217	2843	2854	2873	rVB	86478	137806	4.49%	1.843%
18	11.249	3164	3175	3195	rBV	265794	407563	13.27%	5.450%
19	11.622	3281	3291	3308	rBV	200791	314080	10.23%	4.200%




Sum of corrected areas: 7478077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026401.D
Acq On : 17 Jun 2022 23:40
Operator : SY/MD
Sample : N3278-10 10000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

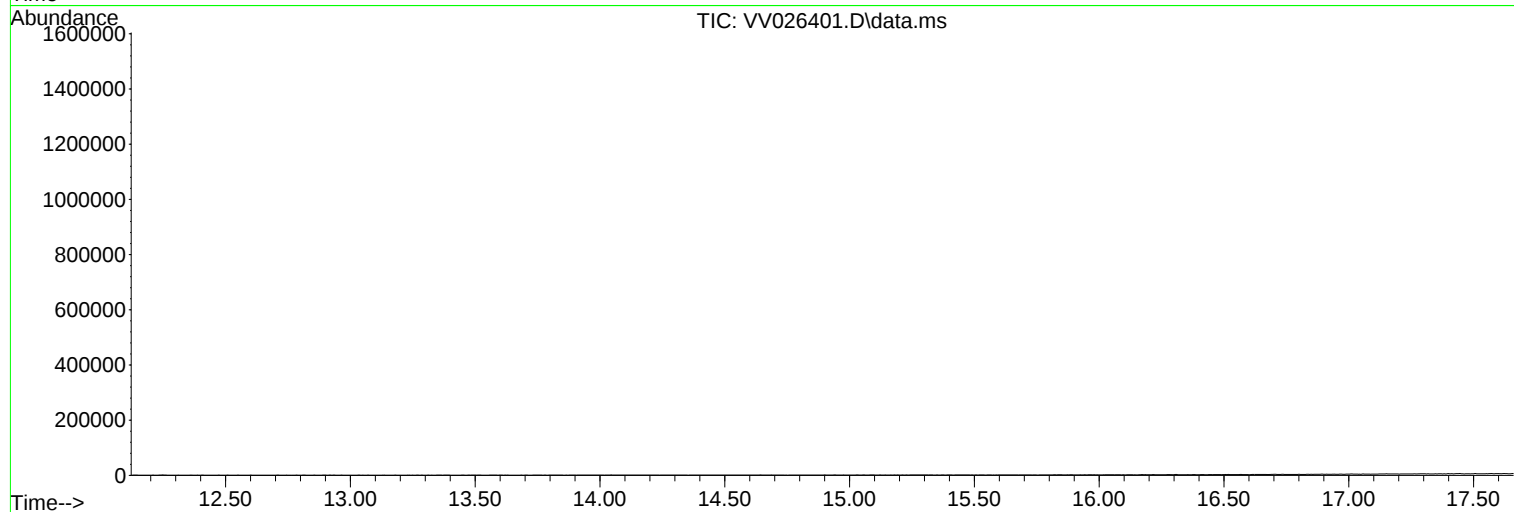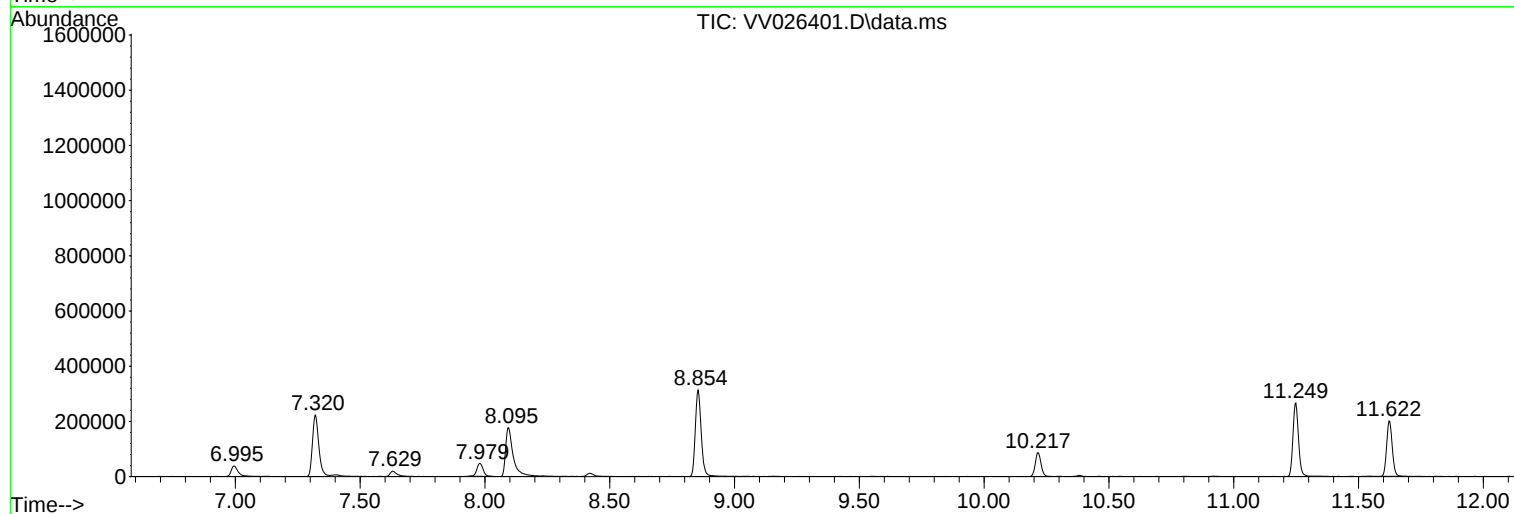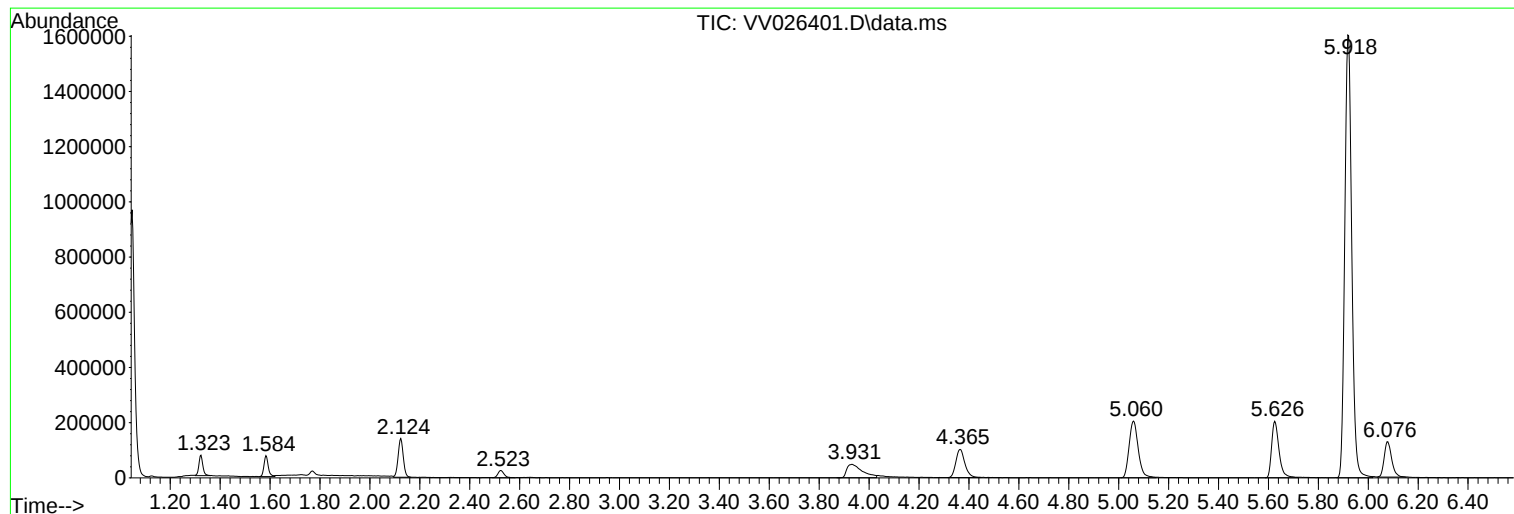

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026401.D
Acq On : 17 Jun 2022 23:40
Operator : SY/MD
Sample : N3278-10 10000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026401.D
Acq On : 17 Jun 2022 23:40
Operator : SY/MD
Sample : N3278-10 10000X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
