

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026408.D
 Acq On : 18 Jun 2022 02:28
 Operator : SY/MD
 Sample : N3358-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4R7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	78	87	101	rVB2	81355	112341	21.94%	2.491%
2	1.433	115	122	129	rVB	42006	46497	9.08%	1.031%
3	1.536	131	154	162	rBV2	56694	234116	45.72%	5.190%
4	1.584	164	169	198	rVB	90689	166683	32.55%	3.695%
5	2.124	328	337	351	rVB	130865	200997	39.25%	4.456%
6	2.310	386	395	406	rVB	19978	31333	6.12%	0.695%
7	3.947	890	904	944	rBV2	23901	125346	24.48%	2.779%
8	4.365	1017	1034	1061	rBV	96346	243970	47.65%	5.409%
9	5.060	1235	1250	1280	rBV4	196570	491802	96.05%	10.903%
10	5.625	1413	1426	1452	rBV	206568	422092	82.43%	9.358%
11	6.076	1551	1566	1593	rBV	117725	250110	48.84%	5.545%
12	6.995	1842	1852	1867	rBV	34059	64771	12.65%	1.436%
13	7.320	1933	1953	1970	rBV	205017	368199	71.91%	8.163%
14	7.400	1970	1978	1997	rVB3	12916	25859	5.05%	0.573%
15	7.632	2041	2050	2080	rBV2	16532	33378	6.52%	0.740%
16	8.095	2183	2194	2230	rBV	151895	340445	66.49%	7.548%
17	8.854	2418	2430	2458	rBV	304080	512051	100.00%	11.352%
18	10.217	2844	2854	2869	rVB	80336	129021	25.20%	2.860%
19	11.249	3162	3175	3196	rBV	267957	413969	80.85%	9.178%
20	11.622	3280	3291	3308	rBV	187629	297685	58.14%	6.600%




Sum of corrected areas: 4510665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026408.D
Acq On : 18 Jun 2022 02:28
Operator : SY/MD
Sample : N3358-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

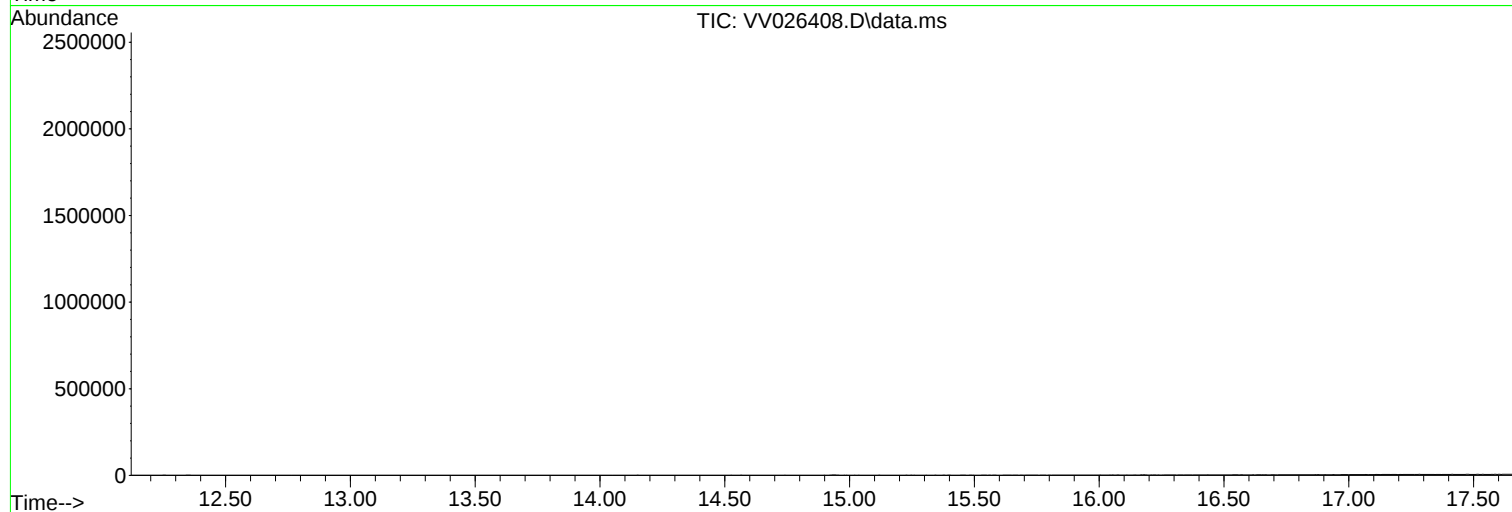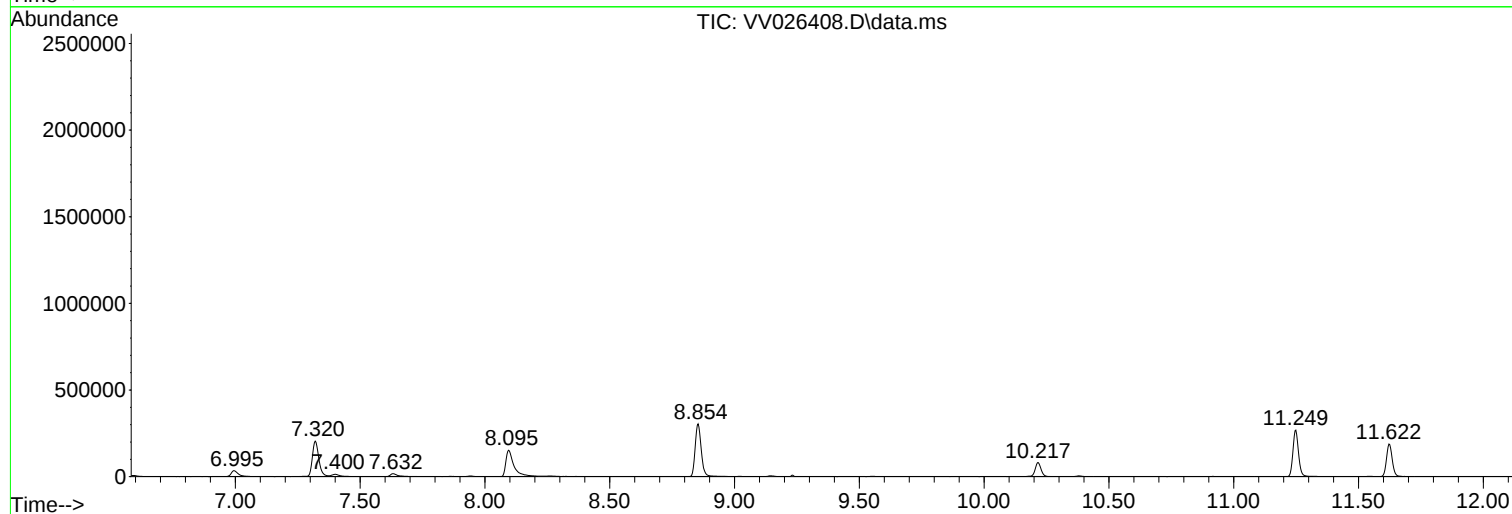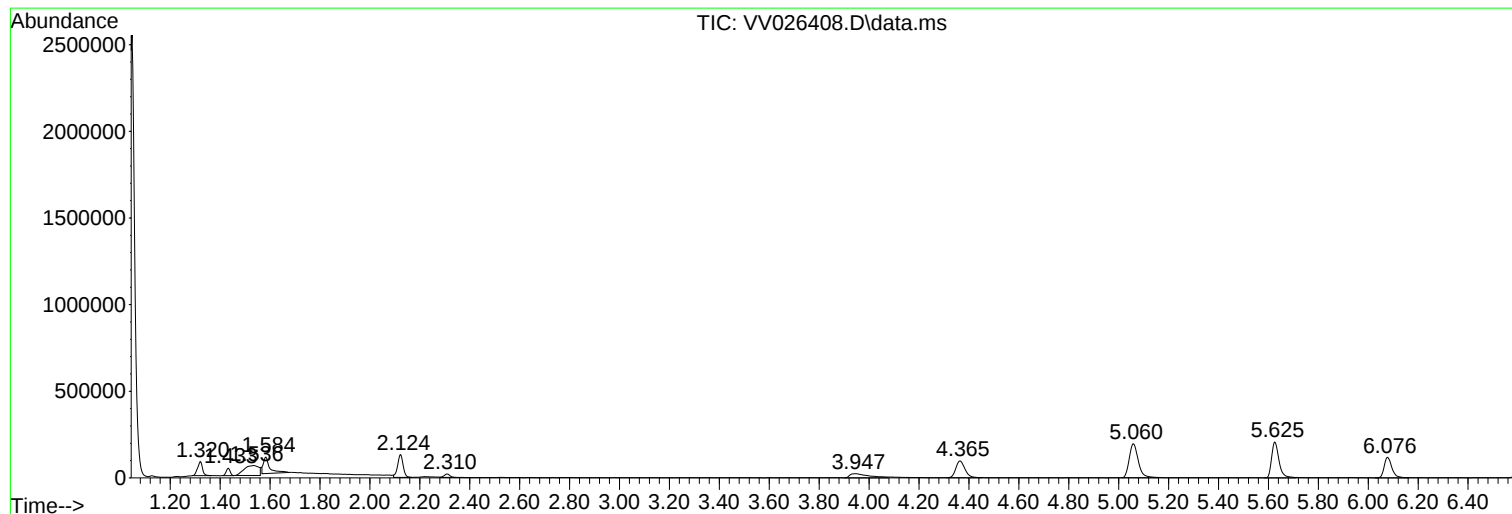

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026408.D
Acq On : 18 Jun 2022 02:28
Operator : SY/MD
Sample : N3358-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
Data File : VV026408.D
Acq On : 18 Jun 2022 02:28
Operator : SY/MD
Sample : N3358-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc