
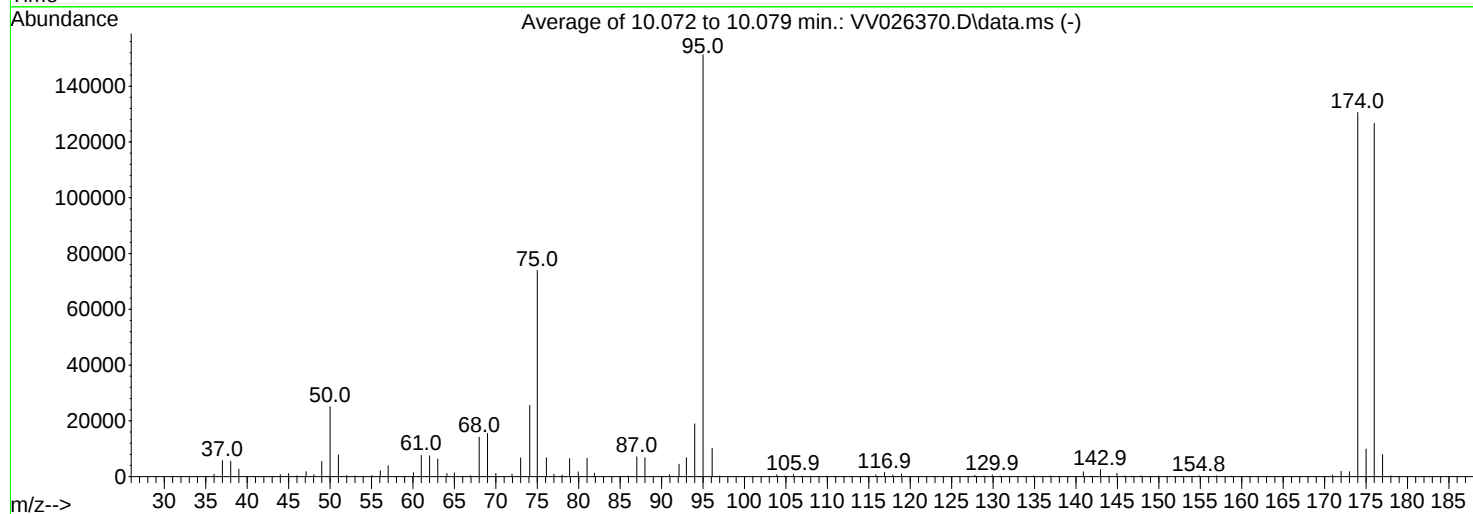


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061722\
 Data File : VV026370.D
 Acq On : 17 Jun 2022 08:37
 Operator : SY/MD
 Sample : BFB331
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB331

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jun 20 01:25:22 2022

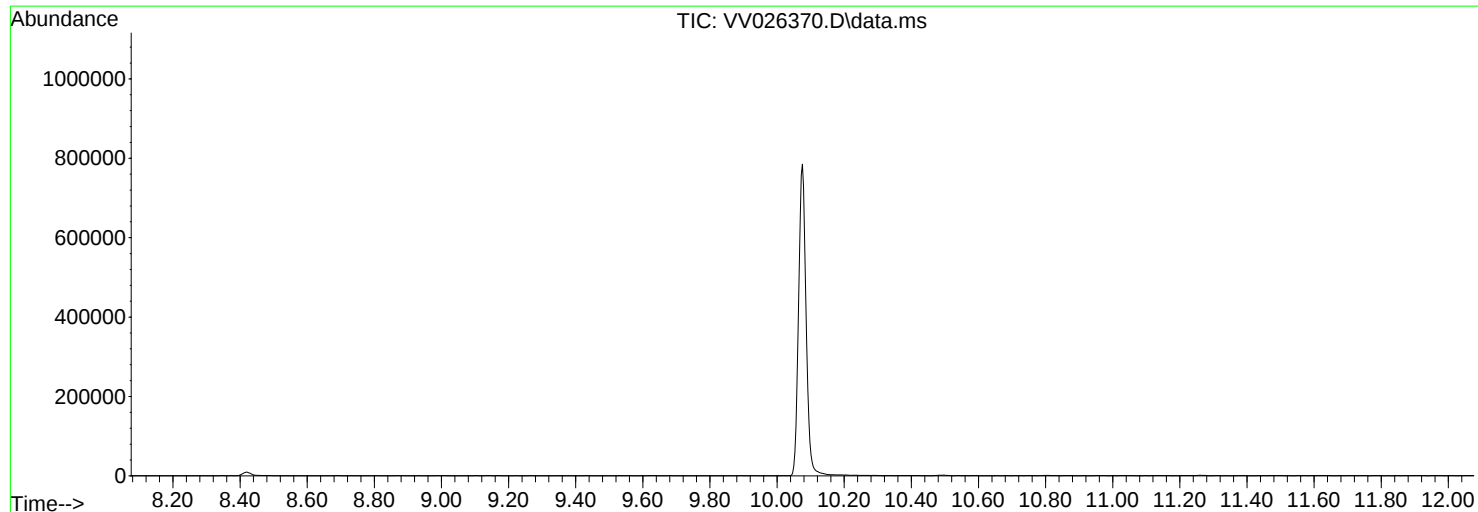

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	25067	PASS
75	95	30	80	48.9	73925	PASS
95	95	100	100	100.0	151232	PASS
96	95	5	9	6.7	10156	PASS
173	174	0.00	2	1.4	1799	PASS
174	95	50	120	86.3	130584	PASS
175	174	5	9	7.6	9902	PASS
176	174	95	105	97.0	126653	PASS
177	176	5	10	6.3	7931	PASS

Scan 2796 (10.030 min): VV026370.D\data.ms
BFB331

m/z	Abundance
39.90	286.0
44.10	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331

m/z	Abundance
36.00	879.0
37.00	5775.0
38.00	5565.0
39.00	2801.0
39.90	328.0
44.00	946.0
45.00	1245.0
46.00	208.0
47.10	1720.0
48.00	746.0
49.00	5596.0
50.00	25448.0
51.00	7882.0
52.00	416.0
53.00	263.0
54.00	124.0
55.00	401.0
56.00	2058.0
57.00	3941.0
57.90	184.0
60.10	1375.0
61.00	7800.0
62.00	7604.0
63.00	6568.0
64.10	1156.0
65.00	1354.0
66.00	116.0
66.90	402.0
68.00	14518.0
69.00	15527.0
70.00	1173.0
72.00	943.0
73.00	6856.0
74.10	25680.0
75.00	74128.0
76.10	6850.0
77.00	837.0
78.00	603.0
78.90	6540.0
80.00	1732.0
81.00	6654.0
81.90	1220.0
82.90	145.0
86.00	265.0
87.00	6947.0
88.00	6829.0
91.00	662.0
92.10	4621.0
93.00	6931.0
94.00	19216.0
95.00	151680.0
96.10	10398.0
97.00	264.0
103.90	656.0
104.80	258.0
105.90	740.0
106.90	136.0
108.00	183.0
109.80	119.0
110.90	165.0
112.00	135.0
112.90	203.0
114.70	162.0
114.90	161.0
115.90	697.0
116.90	1515.0
117.90	659.0
118.90	1013.0
125.90	121.0
127.80	423.0
128.90	237.0
129.90	613.0
130.90	232.0
134.90	245.0
136.90	278.0
139.90	144.0
140.90	1695.0
141.80	235.0
142.90	2596.0
143.90	185.0
145.00	1312.0
145.90	329.0
146.70	189.0
147.80	318.0
148.90	159.0
150.00	206.0
152.80	116.0
153.90	127.0
154.90	394.0
155.80	106.0
156.90	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331

158.80	238.0
160.70	138.0
171.00	660.0
172.00	1789.0
173.00	1774.0
174.00	128272.0
175.00	10233.0
176.00	124768.0
177.00	8191.0
178.00	285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331

m/z	Abundance
36.00	887.0
37.00	5888.0
38.00	5802.0
39.00	2769.0
40.00	330.0
44.00	983.0
45.00	1136.0
46.00	273.0
47.10	1870.0
48.10	749.0
49.00	5644.0
50.00	25912.0
51.00	7991.0
52.00	431.0
53.00	266.0
54.00	125.0
55.00	376.0
56.00	2181.0
57.00	4056.0
58.00	199.0
60.00	1519.0
61.00	8075.0
62.00	7666.0
63.00	6510.0
64.10	1204.0
65.00	1428.0
66.00	156.0
66.90	340.0
68.00	14602.0
69.00	16125.0
70.00	1180.0
71.90	935.0
73.00	6930.0
74.10	26504.0
75.00	76416.0
76.10	6970.0
77.00	890.0
78.00	585.0
78.90	6664.0
80.00	1787.0
81.00	6820.0
81.90	1301.0
83.00	142.0
85.90	202.0
87.00	7381.0
88.00	7068.0
91.00	716.0
92.10	4566.0
93.00	6929.0
94.00	19448.0
95.00	156992.0
96.10	10627.0
97.00	275.0
103.90	710.0
104.90	227.0
105.90	828.0
106.90	163.0
107.90	170.0
109.90	113.0
110.80	162.0
112.00	133.0
112.90	217.0
114.90	197.0
115.90	661.0
116.90	1567.0
117.90	670.0
119.00	976.0
125.90	137.0
127.80	502.0
128.90	249.0
129.90	694.0
130.80	240.0
134.90	295.0
136.90	315.0
139.90	147.0
140.90	1769.0
141.80	257.0
142.90	2558.0
143.90	174.0
145.00	1254.0
145.90	301.0
146.80	155.0
147.80	301.0
148.90	158.0
150.00	238.0
152.80	129.0
154.00	129.0
154.80	328.0
155.70	115.0
156.90	281.0
158.80	249.0
160.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331

171.00	630.0
172.00	1997.0
173.00	1847.0
174.00	135360.0
175.00	10296.0
176.00	131584.0
177.00	8228.0
178.00	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331

m/z	Abundance
36.00	903.0
37.00	5498.0
38.00	5296.0
39.00	2477.0
40.00	330.0
43.20	116.0
44.00	901.0
45.00	942.0
46.00	322.0
47.10	1671.0
48.00	625.0
49.00	5150.0
50.00	23840.0
51.00	7324.0
52.00	378.0
53.00	230.0
54.00	155.0
55.10	377.0
56.10	2062.0
57.00	3698.0
58.00	182.0
60.00	1443.0
61.00	7113.0
62.00	7051.0
63.00	5826.0
64.10	1112.0
65.00	1419.0
66.10	148.0
66.90	266.0
68.00	13441.0
69.00	14758.0
70.00	1043.0
71.90	866.0
73.00	6307.0
74.10	24368.0
75.00	71232.0
76.10	6506.0
77.00	831.0
78.00	541.0
78.90	6165.0
79.90	1682.0
81.00	6354.0
81.90	1272.0
83.00	141.0
85.90	201.0
87.00	6935.0
88.00	6530.0
90.90	630.0
92.10	4156.0
93.00	6435.0
94.00	18136.0
95.00	145024.0
96.10	9444.0
97.00	276.0
103.90	647.0
104.90	166.0
105.90	804.0
106.90	176.0
107.90	144.0
110.00	113.0
110.80	186.0
112.00	119.0
112.90	183.0
114.90	203.0
115.80	583.0
116.90	1453.0
117.90	609.0
119.00	895.0
125.90	106.0
127.80	532.0
128.90	233.0
129.90	625.0
130.90	224.0
134.90	327.0
136.90	296.0
139.90	121.0
140.90	1647.0
141.80	255.0
143.00	2366.0
144.00	181.0
144.90	1115.0
145.90	271.0
146.80	125.0
147.90	276.0
148.90	119.0
149.90	230.0
152.70	113.0
154.10	108.0
154.80	290.0
157.00	298.0
158.80	214.0
160.90	174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331

170.90	515.0
172.00	1930.0
173.00	1775.0
174.00	128120.0
175.00	9176.0
176.00	123608.0
177.00	7375.0
178.00	250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB331