
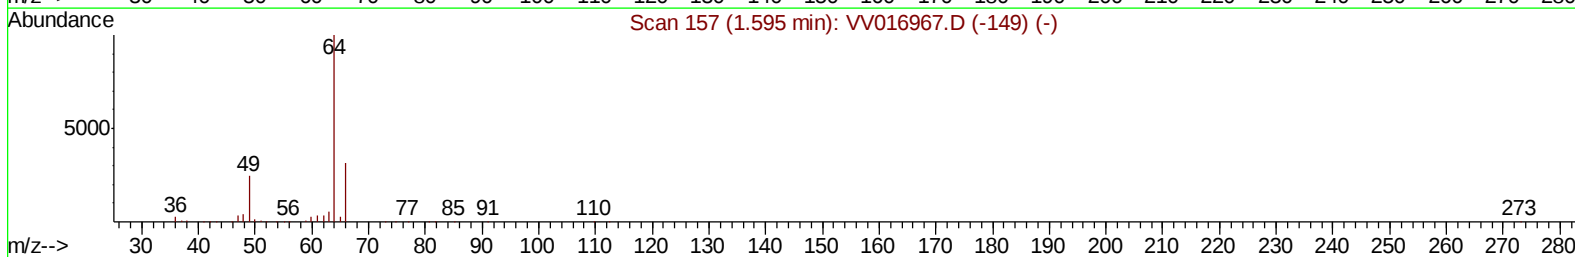
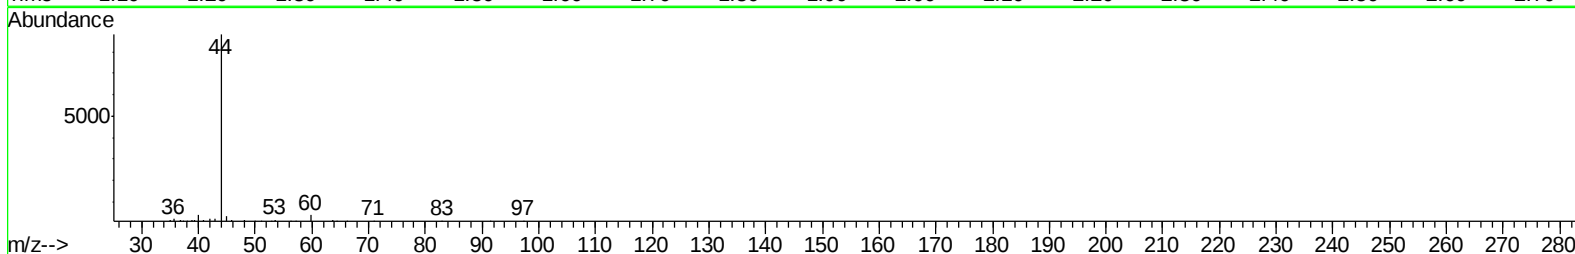


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016971.D
Acq On : 18 Jun 2020 12:04
Operator : SY/MD
Sample : L3039-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 19 05:18:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 19 04:33:43 2020
Response via : Initial Calibration

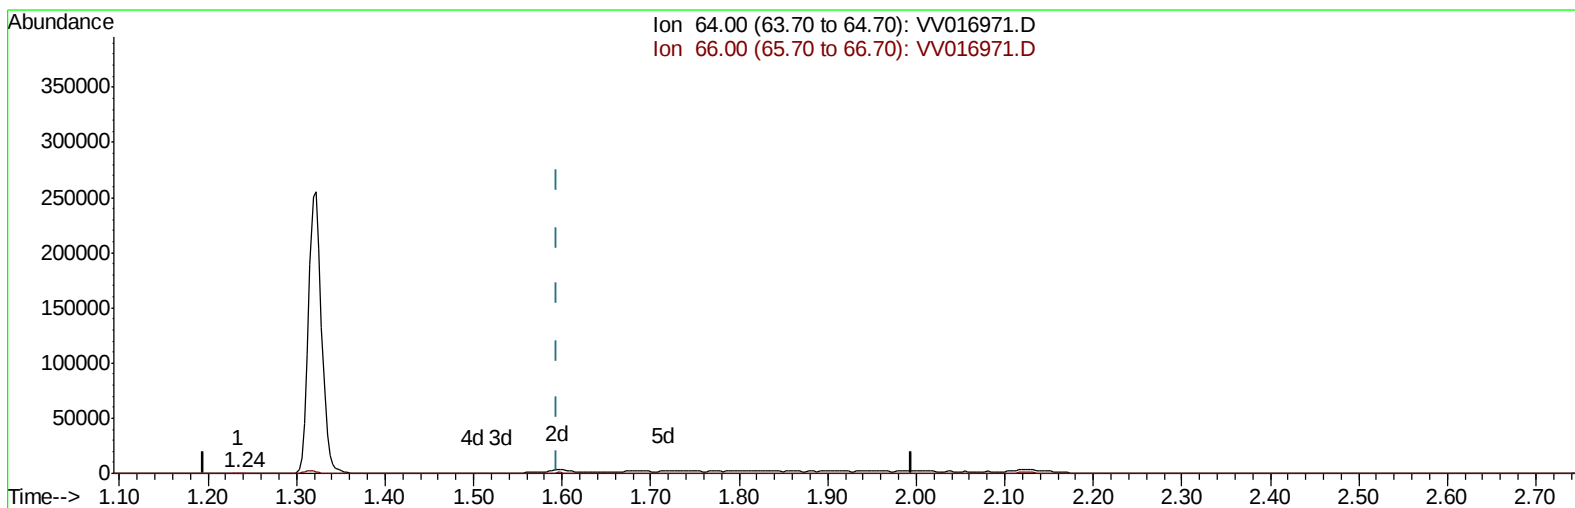

TIC: VV016971.D

(8) Chloroethane (T)

1.235min (-0.360) 0.12ug/L

response 167

Ion	Exp%	Act%
64.00	100	100
66.00	33.10	34.45
0.00	0.00	0.00
0.00	0.00	0.00