
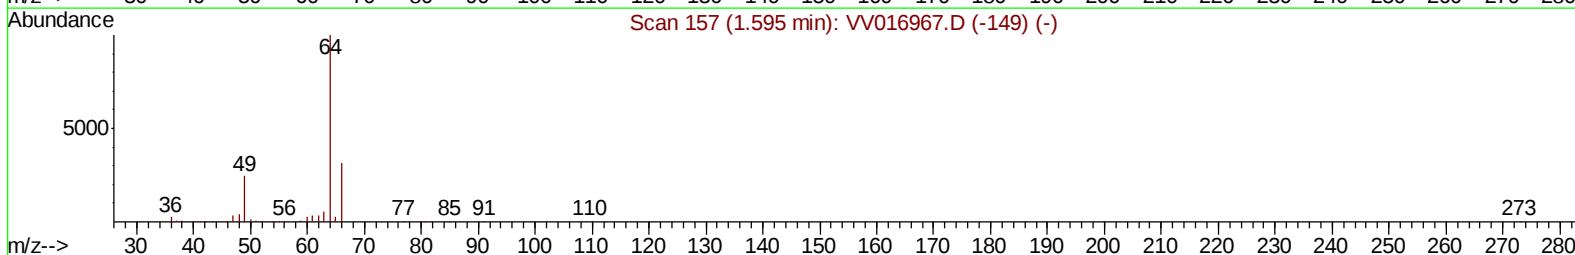
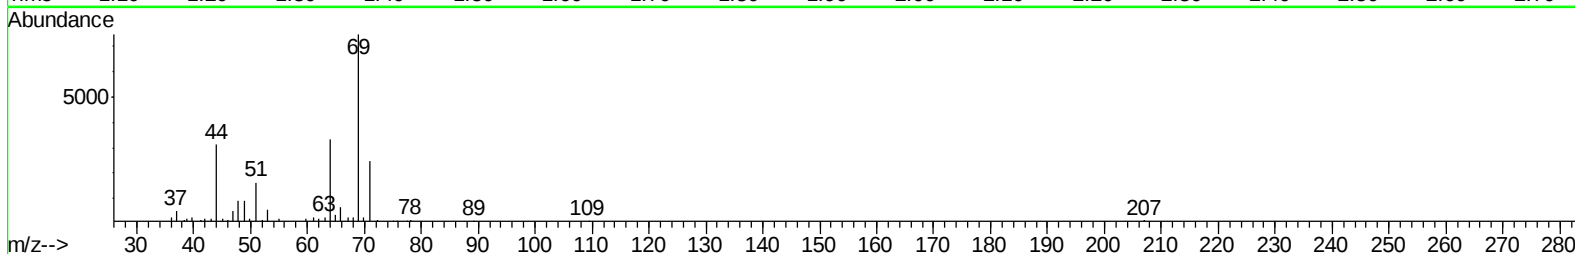


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016971.D
 Acq On : 18 Jun 2020 12:04
 Operator : SY/MD
 Sample : L3039-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 19 05:18:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 19 04:33:43 2020
 Response via : Initial Calibration

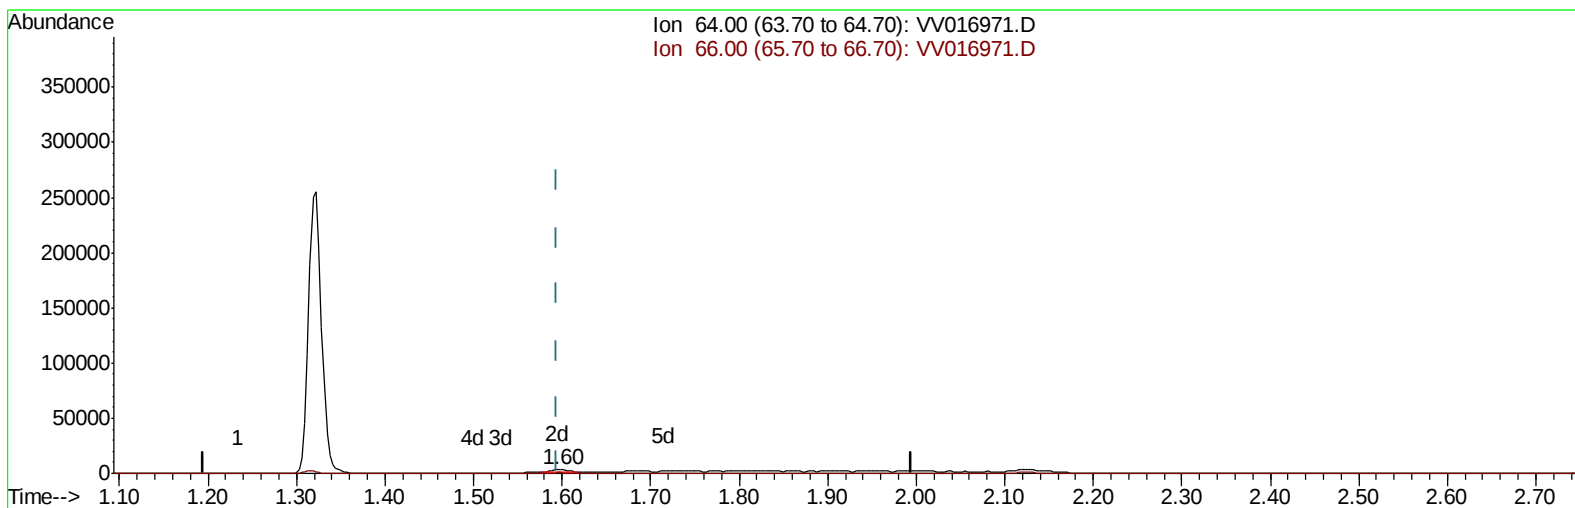

TIC: VV016971.D

(8) Chloroethane (T)

1.595min (+0.000) 2.92ug/L m

response 3908

Ion	Exp%	Act%
64.00	100	100
66.00	33.10	19.35#
0.00	0.00	0.00
0.00	0.00	0.00