
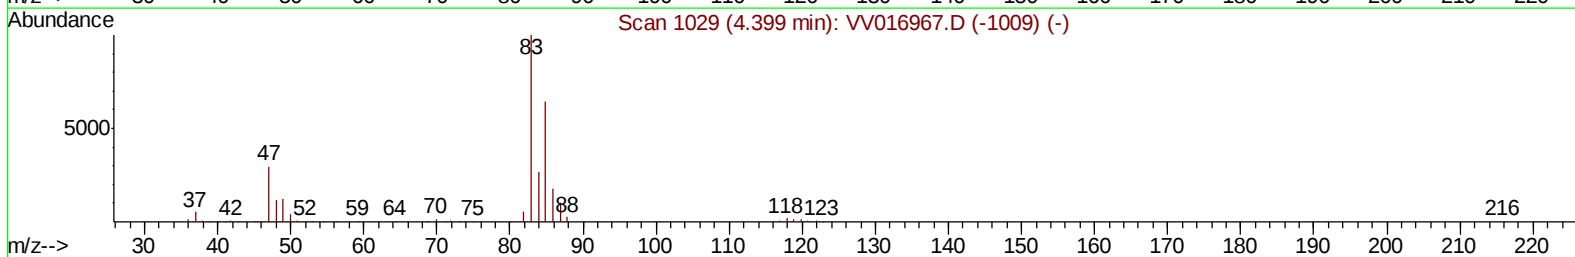
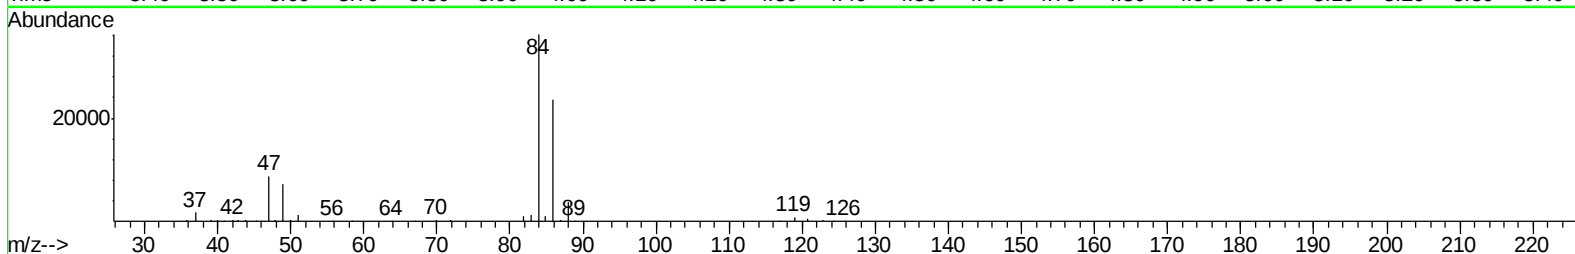


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\  
Data File : VV016980.D  
Acq On : 18 Jun 2020 15:33  
Operator : SY/MD  
Sample : L3039-09  
Misc : 5.0mL/MSVOA V/WATER  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jun 19 04:37:59 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM060820WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Jun 19 04:33:43 2020  
Response via : Initial Calibration

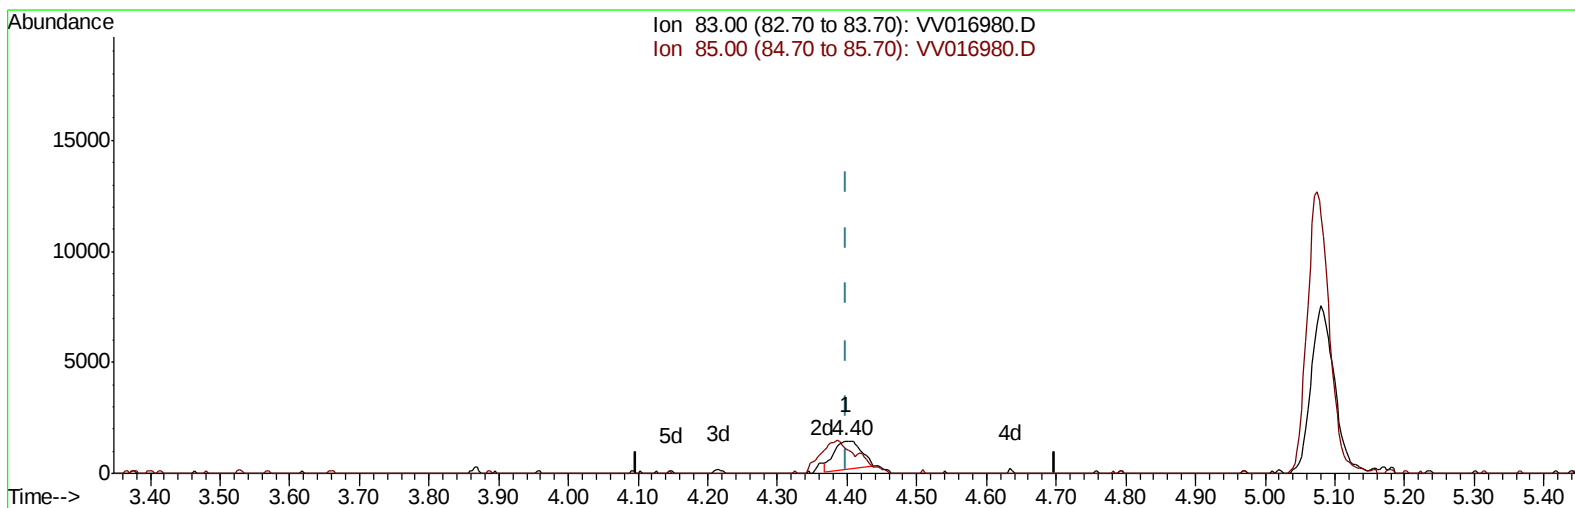

TIC: VV016980.D

(25) Chloroform (T)

4.399min (+0.000) 0.78ug/L

response 3582

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 83.00 | 100   | 100   |
| 85.00 | 63.00 | 75.27 |
| 0.00  | 0.00  | 0.00  |
| 0.00  | 0.00  | 0.00  |