
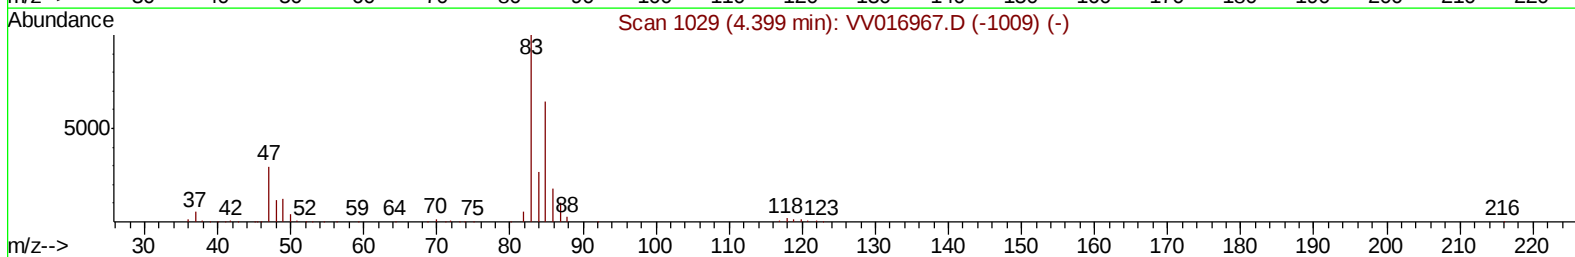
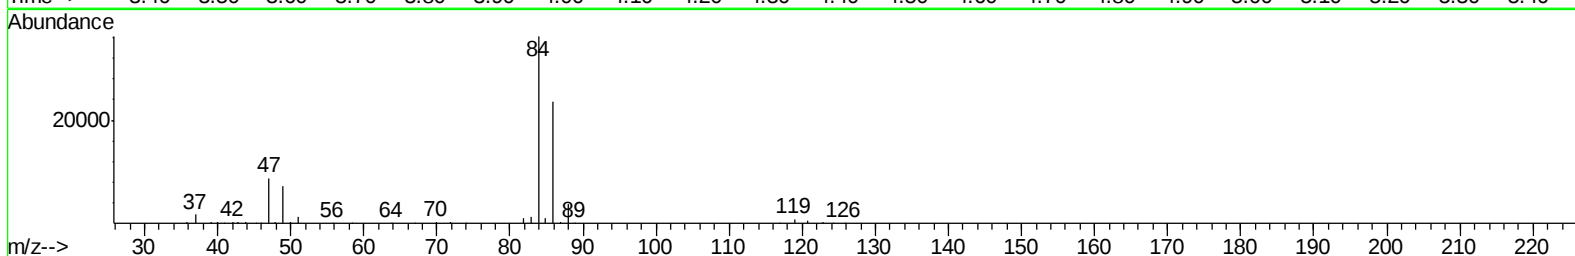


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016980.D
Acq On : 18 Jun 2020 15:33
Operator : SY/MD
Sample : L3039-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jun 19 04:37:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 19 04:33:43 2020
Response via : Initial Calibration

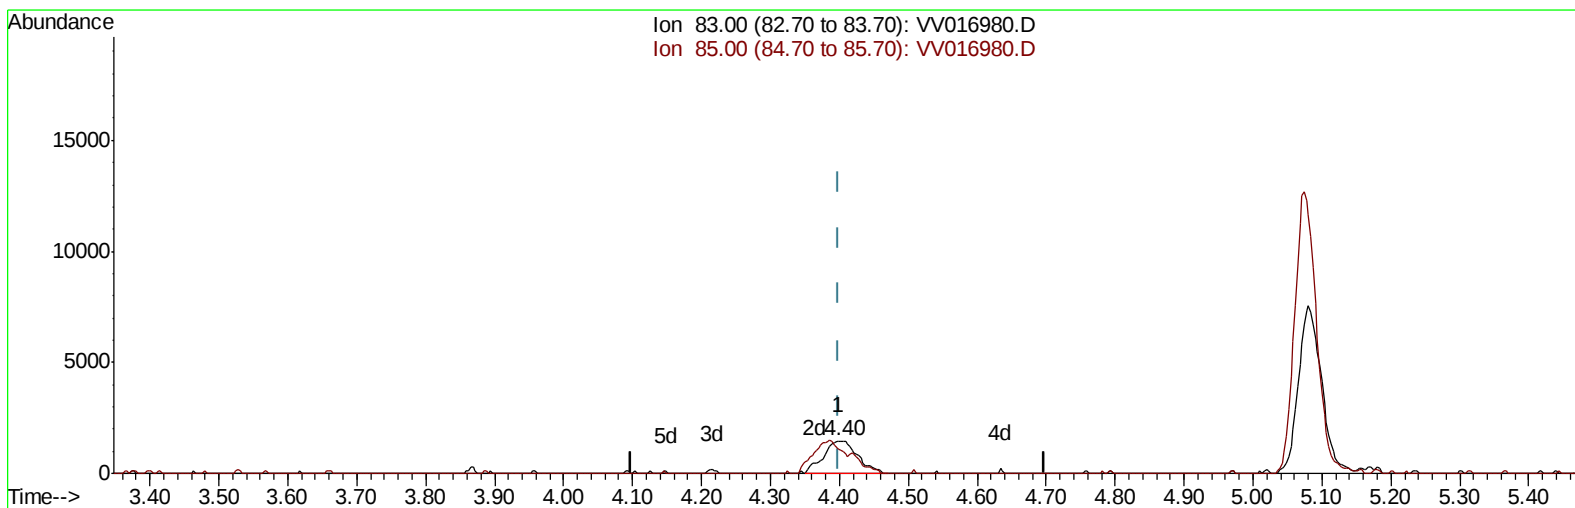

TIC: VV016980.D

(25) Chloroform (T)

4.399min (+0.000) 1.09ug/L m

response 5041

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	75.27
0.00	0.00	0.00
0.00	0.00	0.00