
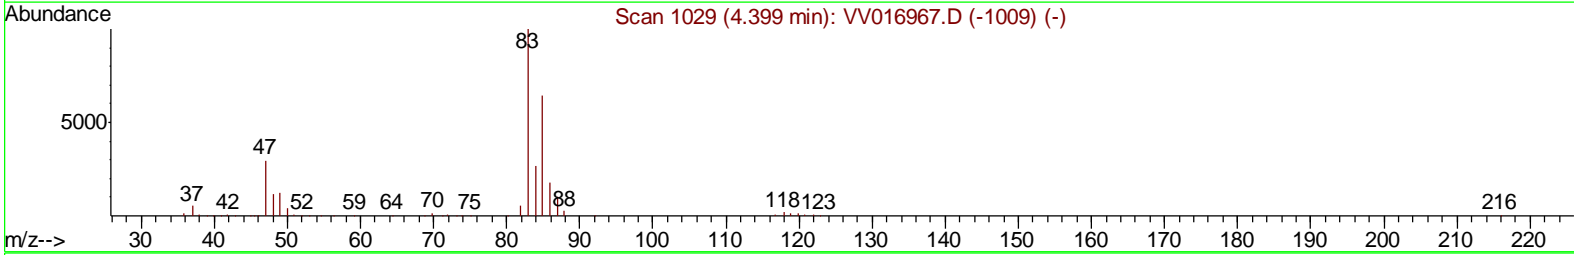
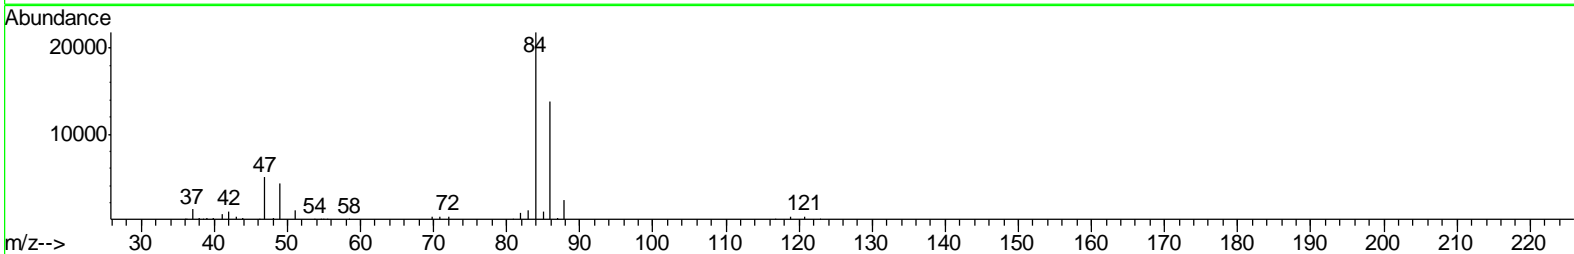


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016981.D
 Acq On : 18 Jun 2020 15:56
 Operator : SY/MD
 Sample : L3039-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 19 04:38:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 19 04:33:43 2020
 Response via : Initial Calibration

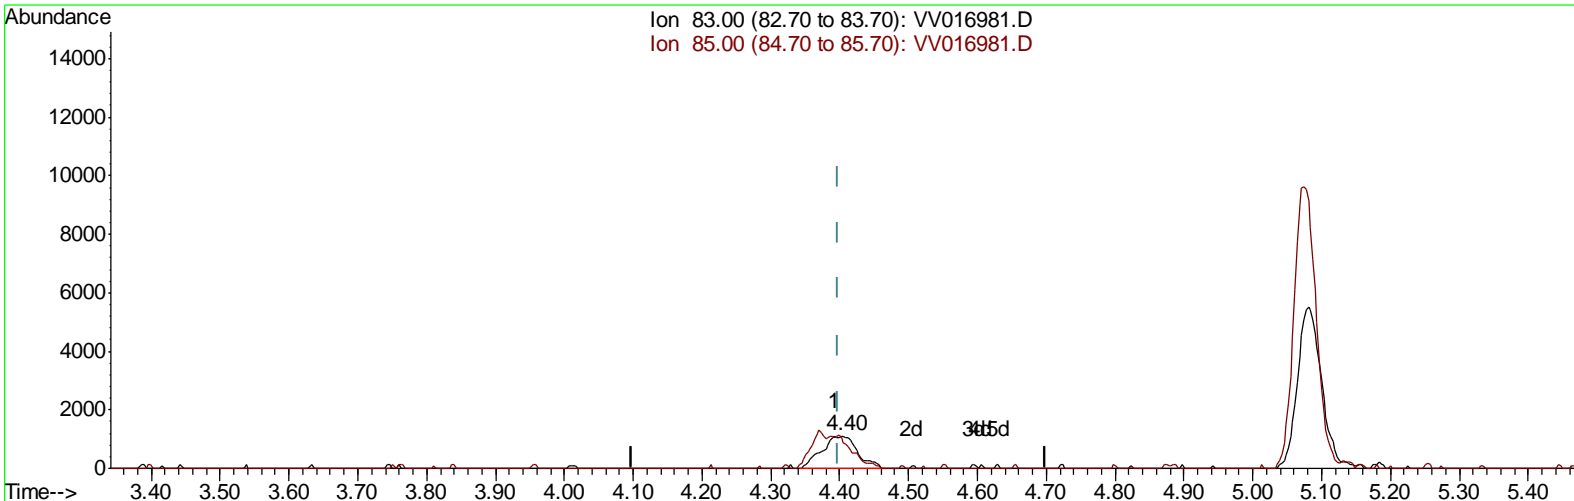

TIC: VV016981.D

(25) Chloroform (T)
 4.402min (+0.003) 1.14ug/L m
 response 3994

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	93.25#
0.00	0.00	0.00
0.00	0.00	0.00