
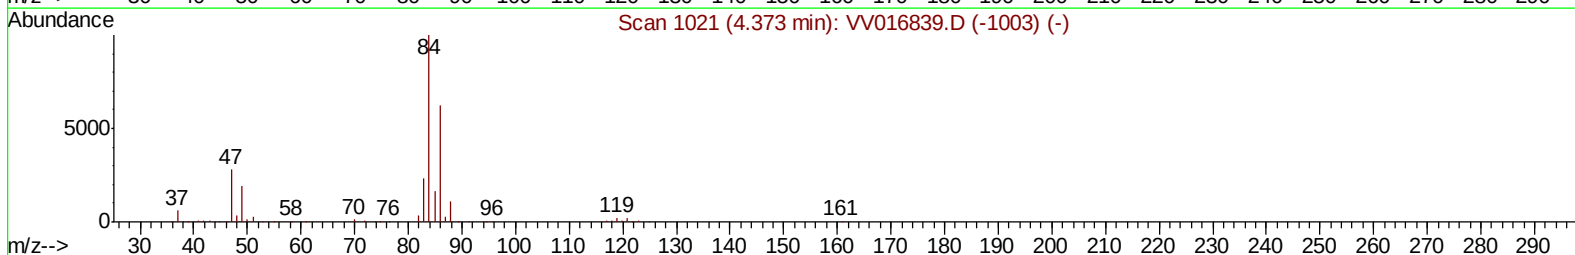
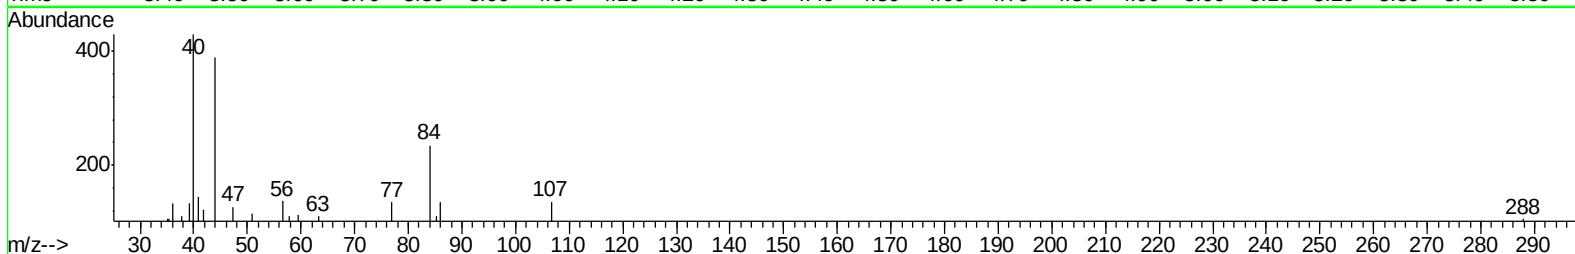


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016986.D
 Acq On : 18 Jun 2020 18:38
 Operator : SY/MD
 Sample : L3039-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 19 04:39:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 19 04:33:43 2020
 Response via : Initial Calibration

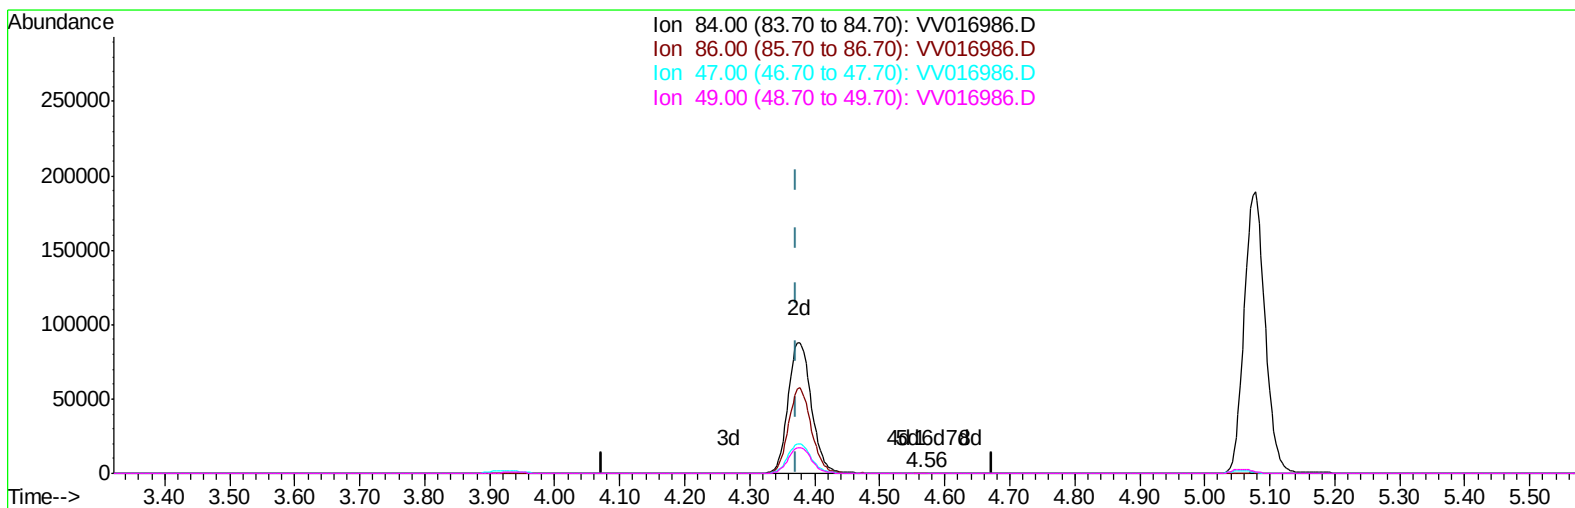

TIC: VV016986.D

(24) Chloroform-d (S)

4.563min (+0.190) 0.04ug/L

response 208

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	45.19
47.00	44.50	49.04
49.00	27.40	31.25