


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016972.D
Acq On : 18 Jun 2020 12:28
Operator : SY/MD
Sample : L3039-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M02

Manual Integrations
APPROVED

MMDadoda
6/19/2020 3:02:37 PM

Quant Time: Jun 19 05:34:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 19 04:33:43 2020
Response via : Initial Calibration

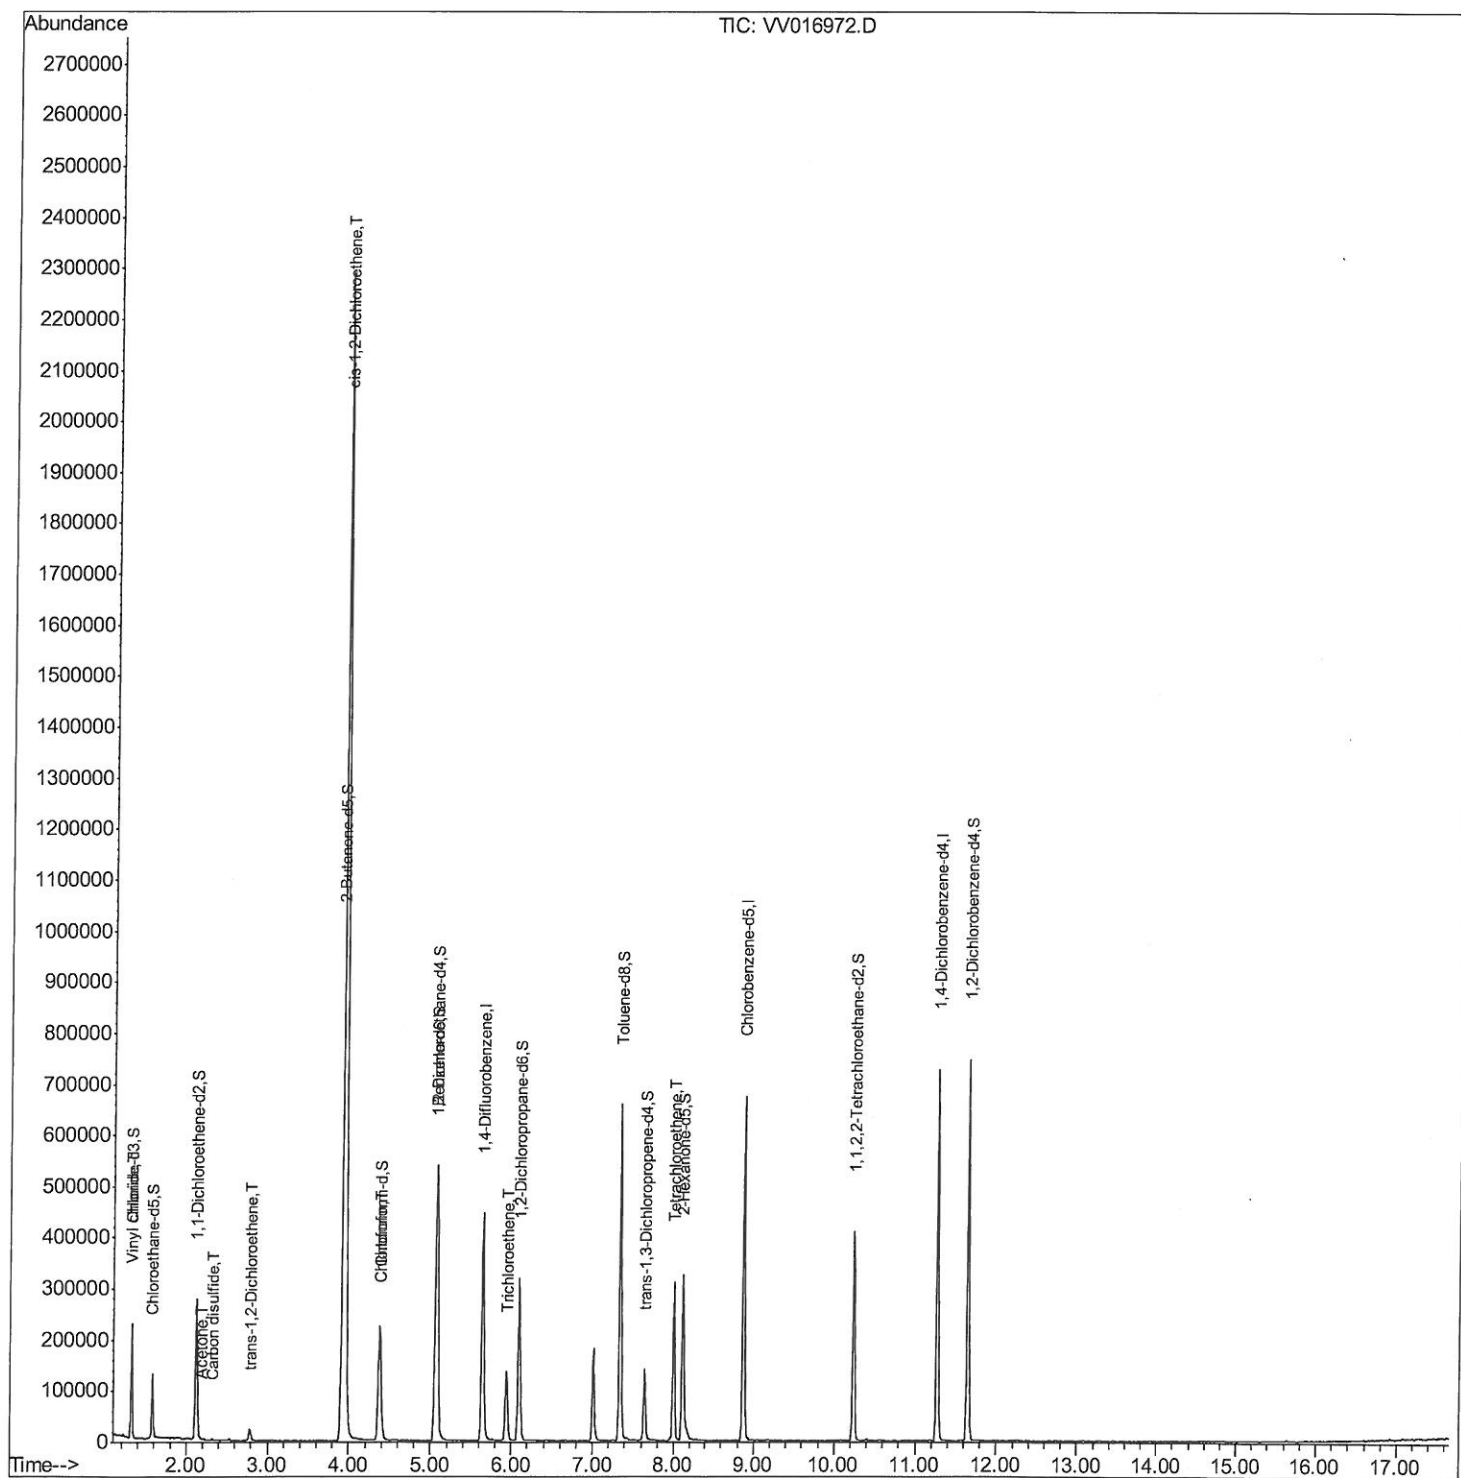

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016972.D
 Acq On : 18 Jun 2020 12:28
 Operator : SY/MD
 Sample : L3039-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 F9M02

Manual Integrations
APPROVED

MMDadoda
 6/19/2020 3:02:37 PM

Quant Time: Jun 19 04:36:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 19 04:33:43 2020
 Response via : Initial Calibration

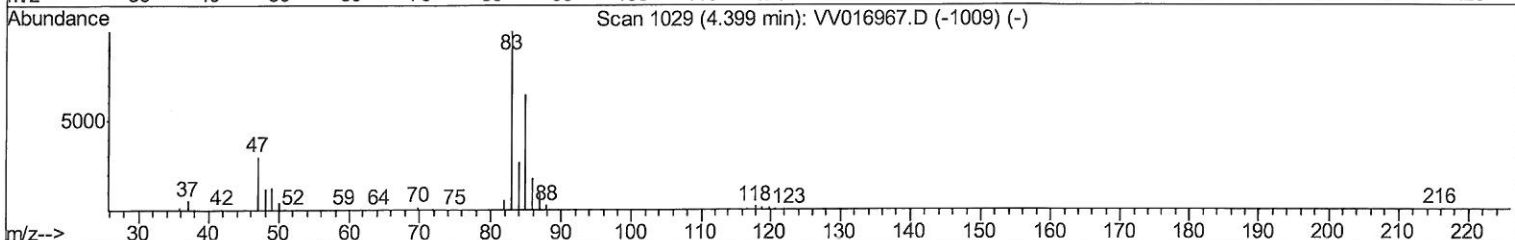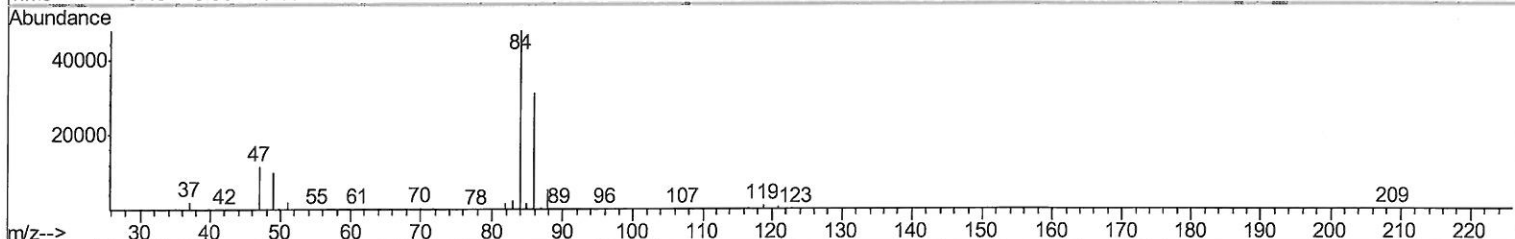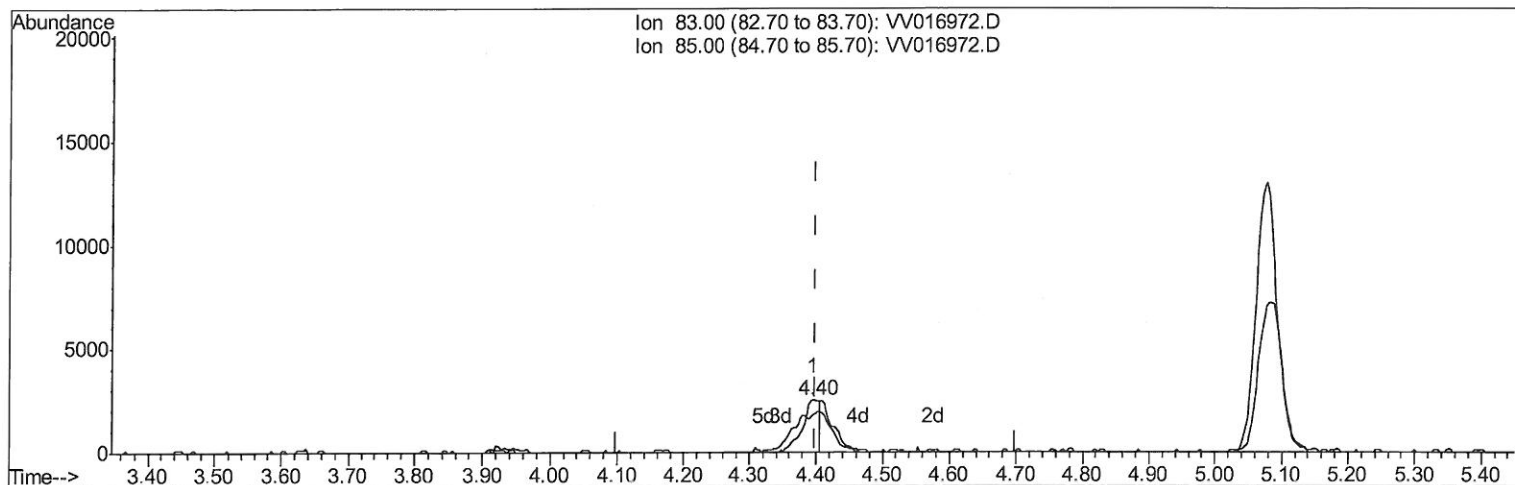

TIC: VV016972.D

(25) Chloroform (T)

4.396min (-0.003) 0.93ug/L

response 4486

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	73.52
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016972.D
 Acq On : 18 Jun 2020 12:28
 Operator : SY/MD
 Sample : L3039-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 F9M02

Manual Integrations
 APPROVED

MMDadoda
 6/19/2020 3:02:37 PM

Quant Time: Jun 19 04:36:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 19 04:33:43 2020
 Response via : Initial Calibration

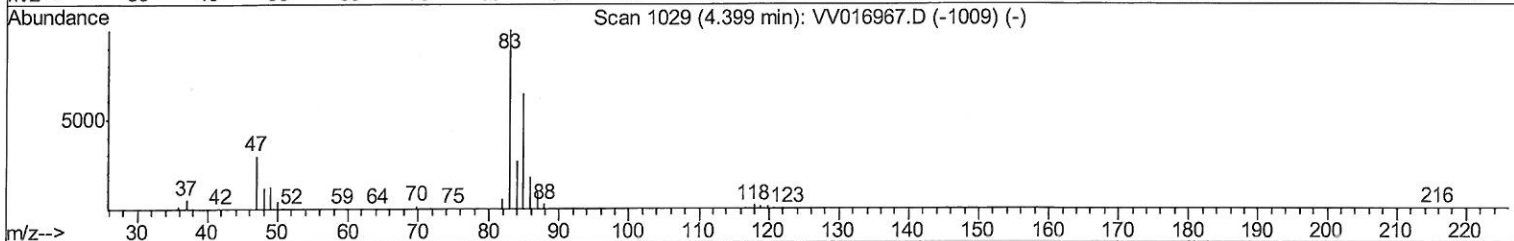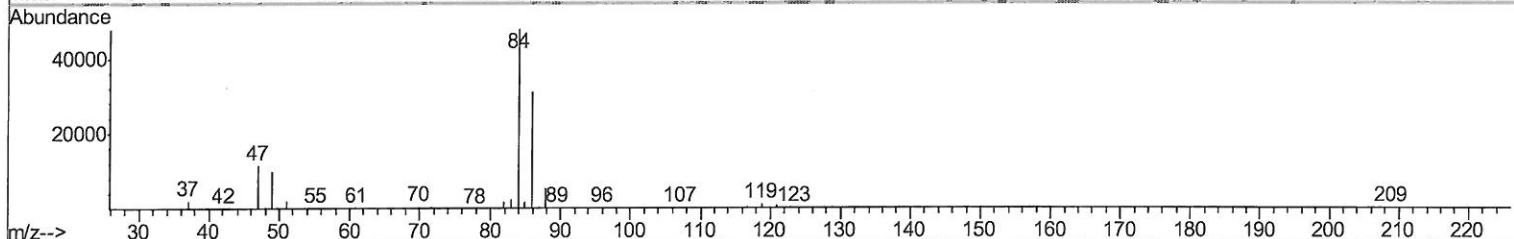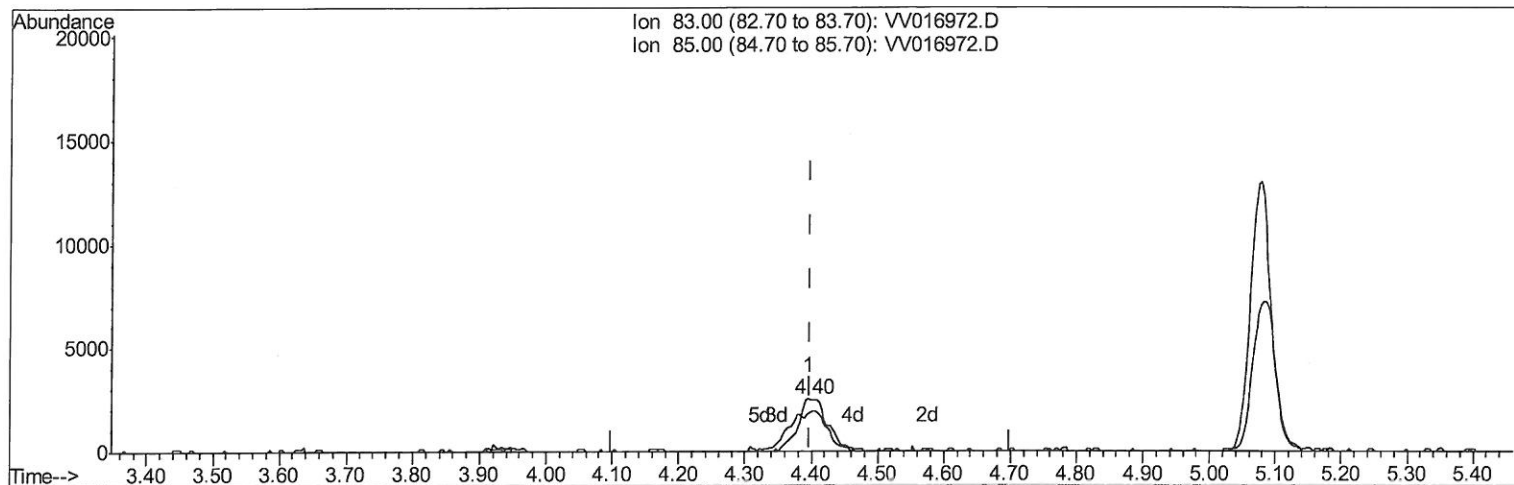

TIC: VV016972.D

(25) Chloroform (T)

4.396min (-0.003) 1.61ug/L m

response 7742

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	73.52
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 06/23/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016972.D
 Acq On : 18 Jun 2020 12:28
 Operator : SY/MD
 Sample : L3039-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M02

Manual Integrations
 APPROVED

MMDadoda
 6/19/2020 3:02:37 PM

Quant Time: Jun 19 05:34:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 19 04:33:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	367814	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	356177	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	180523	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	93590	36.06	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.12%		
7) Chloroethane-d5	1.58	69	71823	46.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.24%		
11) 1,1-Dichloroethene-d2	2.13	63	146310	33.57	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.14%		
21) 2-Butanone-d5	3.91	46	170961	89.00	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.00%		
24) Chloroform-d	4.38	84	226827	42.98	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.96%		
26) 1,2-Dichloroethane-d4	5.06	65	167118	46.56	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.12%		
32) Benzene-d6	5.08	84	445945	43.43	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.86%		
36) 1,2-Dichloropropane-d6	6.09	67	138920	43.41	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.82%		
41) Toluene-d8	7.34	98	416737	44.23	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.46%		
43) trans-1,3-Dichloropropene-	7.64	79	71650	42.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.96%		
47) 2-Hexanone-d5	8.11	63	102187	73.24	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	73.24%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	183588	43.33	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.66%		
64) 1,2-Dichlorobenzene-d4	11.65	152	184425	47.87	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.74%		
Target Compounds						
5) Vinyl chloride	1.32	62	49073	18.713	ug/L	93
13) Acetone	2.19	43	3657	2.889	ug/L	89
14) Carbon disulfide	2.31	76	3972	0.601	ug/L #	80
17) trans-1,2-Dichloroethene	2.78	96	8457	3.398	ug/L	98
20) cis-1,2-Dichloroethene	3.94	96	1247979	459.903	ug/L	98
25) Chloroform	4.40	83	7742m	1.608	ug/L	98
34) Trichloroethene	5.94	95	44537	15.758	ug/L	98
46) Tetrachloroethene	8.00	164	67174	30.220	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed