

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016970.D
 Acq On : 18 Jun 2020 11:41
 Operator : SY/MD
 Sample : L3039-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	88	rVB2	1385835	1435916	34.01%	8.914%
2	1.576	145	151	167	rVB	122608	143687	3.40%	0.892%
3	2.122	312	321	338	rVB	268701	397623	9.42%	2.468%
4	3.036	602	605	606	rBV3	1366	553	0.01%	0.003%
5	3.068	613	615	617	rBV3	1263	675	0.02%	0.004%
6	3.106	625	627	629	rBV3	1034	562	0.01%	0.003%
7	3.293	683	685	688	rBV3	1500	878	0.02%	0.005%
8	3.393	714	716	717	rBV	1506	605	0.01%	0.004%
9	3.605	780	782	787	rVB6	1740	1156	0.03%	0.007%
10	3.634	787	791	792	rBV3	1559	1110	0.03%	0.007%
11	3.936	865	885	913	rBV2	1668359	4222056	100.00%	26.210%
12	4.376	1008	1022	1045	rVB	221187	557557	13.21%	3.461%
13	4.605	1091	1093	1096	rBV3	1967	1094	0.03%	0.007%
14	4.627	1099	1100	1101	rBV	1390	403	0.01%	0.003%
15	4.733	1129	1133	1135	rVB4	2027	1304	0.03%	0.008%
16	4.749	1135	1138	1139	rBV2	1565	921	0.02%	0.006%
17	4.910	1186	1188	1190	rVB2	1079	403	0.01%	0.003%
18	4.929	1192	1194	1197	rBV2	1017	451	0.01%	0.003%
19	4.968	1201	1206	1208	rBV4	1733	1386	0.03%	0.009%
20	4.987	1210	1212	1213	rBV2	884	435	0.01%	0.003%
21	5.071	1219	1238	1273	rBV2	540468	1419094	33.61%	8.809%
22	5.299	1308	1309	1310	rBV	1205	330	0.01%	0.002%
23	5.389	1333	1337	1340	rBV5	1684	1526	0.04%	0.009%
24	5.569	1389	1393	1395	rBV4	1662	1565	0.04%	0.010%
25	5.640	1403	1415	1441	rBV	423219	839973	19.89%	5.214%
26	5.933	1497	1506	1530	rVB9	29020	73062	1.73%	0.454%
27	6.093	1543	1556	1581	rBV	311336	628417	14.88%	3.901%
28	6.315	1622	1625	1628	rBV6	1740	1270	0.03%	0.008%
29	6.335	1628	1631	1632	rBV2	1444	819	0.02%	0.005%
30	6.431	1659	1661	1663	rBV3	650	364	0.01%	0.002%
31	6.479	1672	1676	1679	rBV6	2230	1813	0.04%	0.011%
32	6.553	1695	1699	1703	rBV5	1559	1358	0.03%	0.008%
33	6.724	1750	1752	1754	rBV2	986	696	0.02%	0.004%
34	6.904	1806	1808	1811	rBV3	818	494	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016970.D
 Acq On : 18 Jun 2020 11:41
 Operator : SY/MD
 Sample : L3039-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.007	1827	1840	1861	rBV	189276	337046	7.98%	2.092%
36	7.174	1889	1892	1894	rBV5	999	602	0.01%	0.004%
37	7.216	1903	1905	1907	rBV3	1353	584	0.01%	0.004%
38	7.267	1915	1921	1925	rBV8	2167	2547	0.06%	0.016%
39	7.338	1931	1943	1959	rBV	656224	1127835	26.71%	7.001%
40	7.640	2027	2037	2056	rBV2	142968	245359	5.81%	1.523%
41	7.881	2110	2112	2115	rBV3	1326	777	0.02%	0.005%
42	7.897	2115	2117	2120	rBV3	1272	729	0.02%	0.005%
43	7.961	2129	2137	2141	rBV3	7993	12542	0.30%	0.078%
44	8.106	2172	2182	2212	rBV2	310834	615487	14.58%	3.821%
45	8.450	2287	2289	2290	rBV2	1105	511	0.01%	0.003%
46	8.482	2297	2299	2301	rBV3	1119	441	0.01%	0.003%
47	8.556	2318	2322	2324	rBV4	1322	900	0.02%	0.006%
48	8.569	2324	2326	2328	rBV3	1514	632	0.01%	0.004%
49	8.685	2360	2362	2363	rBV	1096	495	0.01%	0.003%
50	8.788	2392	2394	2395	rBV2	1062	341	0.01%	0.002%
51	8.871	2407	2420	2440	rBV	650468	1061553	25.14%	6.590%
52	9.122	2496	2498	2501	rBV4	1596	1267	0.03%	0.008%
53	9.164	2504	2511	2521	rVB	23154	35791	0.85%	0.222%
54	9.273	2542	2545	2547	rBV3	1296	928	0.02%	0.006%
55	9.305	2553	2555	2558	rVB4	1103	594	0.01%	0.004%
56	9.328	2558	2562	2563	rBV4	1943	1392	0.03%	0.009%
57	9.457	2598	2602	2603	rBV4	1241	954	0.02%	0.006%
58	9.572	2628	2638	2647	rBV3	10580	19136	0.45%	0.119%
59	9.669	2665	2668	2671	rBV4	1139	755	0.02%	0.005%
60	9.688	2671	2674	2676	rVB4	1631	732	0.02%	0.005%
61	9.772	2694	2700	2702	rBV7	1654	1847	0.04%	0.011%
62	9.797	2706	2708	2713	rBV5	1947	1675	0.04%	0.010%
63	9.926	2746	2748	2750	rBV3	999	579	0.01%	0.004%
64	10.093	2798	2800	2803	rBV4	1225	444	0.01%	0.003%
65	10.180	2825	2827	2830	rBV4	1490	883	0.02%	0.005%
66	10.238	2834	2845	2865	rVB	406876	637224	15.09%	3.956%
67	10.357	2881	2882	2884	rBV2	1110	507	0.01%	0.003%
68	10.531	2934	2936	2937	rBV2	974	492	0.01%	0.003%
69	10.543	2937	2940	2941	rVV2	1648	870	0.02%	0.005%
70	10.704	2988	2990	2992	rBV3	726	487	0.01%	0.003%
71	10.875	3037	3043	3044	rBV5	2009	1621	0.04%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016970.D
 Acq On : 18 Jun 2020 11:41
 Operator : SY/MD
 Sample : L3039-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.939	3057	3063	3065	rBV7	3588	4047	0.10%	0.025%
73	11.032	3089	3092	3093	rBV2	832	453	0.01%	0.003%
74	11.051	3096	3098	3100	rBV3	1089	611	0.01%	0.004%
75	11.196	3141	3143	3144	rBV2	1681	699	0.02%	0.004%
76	11.270	3155	3166	3183	rBV	695461	1068098	25.30%	6.631%
77	11.389	3201	3203	3206	rVB4	1845	690	0.02%	0.004%
78	11.646	3272	3283	3301	rBV	738293	1143917	27.09%	7.101%
79	11.810	3330	3334	3335	rBV3	2016	1164	0.03%	0.007%
80	11.993	3388	3391	3393	rBV4	1755	1167	0.03%	0.007%
81	12.026	3398	3401	3404	rBV4	1533	1185	0.03%	0.007%
82	12.129	3431	3433	3434	rBV	1827	755	0.02%	0.005%
83	12.167	3439	3445	3449	rBV8	2017	2477	0.06%	0.015%
84	12.235	3462	3466	3468	rBV4	1104	799	0.02%	0.005%
85	12.405	3517	3519	3520	rBV2	1385	516	0.01%	0.003%
86	12.521	3553	3555	3557	rBV2	1237	713	0.02%	0.004%
87	12.611	3581	3583	3587	rVB4	1638	1001	0.02%	0.006%
88	12.772	3631	3633	3637	rBV3	1219	618	0.01%	0.004%
89	12.820	3644	3648	3650	rBV3	1708	1386	0.03%	0.009%
90	12.855	3650	3659	3668	rVV10	7261	12761	0.30%	0.079%
91	13.058	3721	3722	3725	rBV4	1001	584	0.01%	0.004%
92	13.077	3725	3728	3731	rBV4	1920	1406	0.03%	0.009%
93	13.122	3737	3742	3746	rBV7	1702	1092	0.03%	0.007%
94	13.238	3775	3778	3781	rBV5	1342	944	0.02%	0.006%
95	13.743	3933	3935	3938	rBV3	1353	626	0.01%	0.004%
96	13.762	3939	3941	3944	rBV4	1867	919	0.02%	0.006%
97	13.855	3966	3970	3972	rBV4	1138	969	0.02%	0.006%
98	14.286	4101	4104	4108	rBV4	1354	1049	0.02%	0.007%
99	14.331	4116	4118	4122	rBV4	1226	735	0.02%	0.005%
100	14.411	4139	4143	4145	rBV5	1275	1236	0.03%	0.008%


Sum of corrected areas: 16108732

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016970.D
Acq On : 18 Jun 2020 11:41
Operator : SY/MD
Sample : L3039-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M00

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

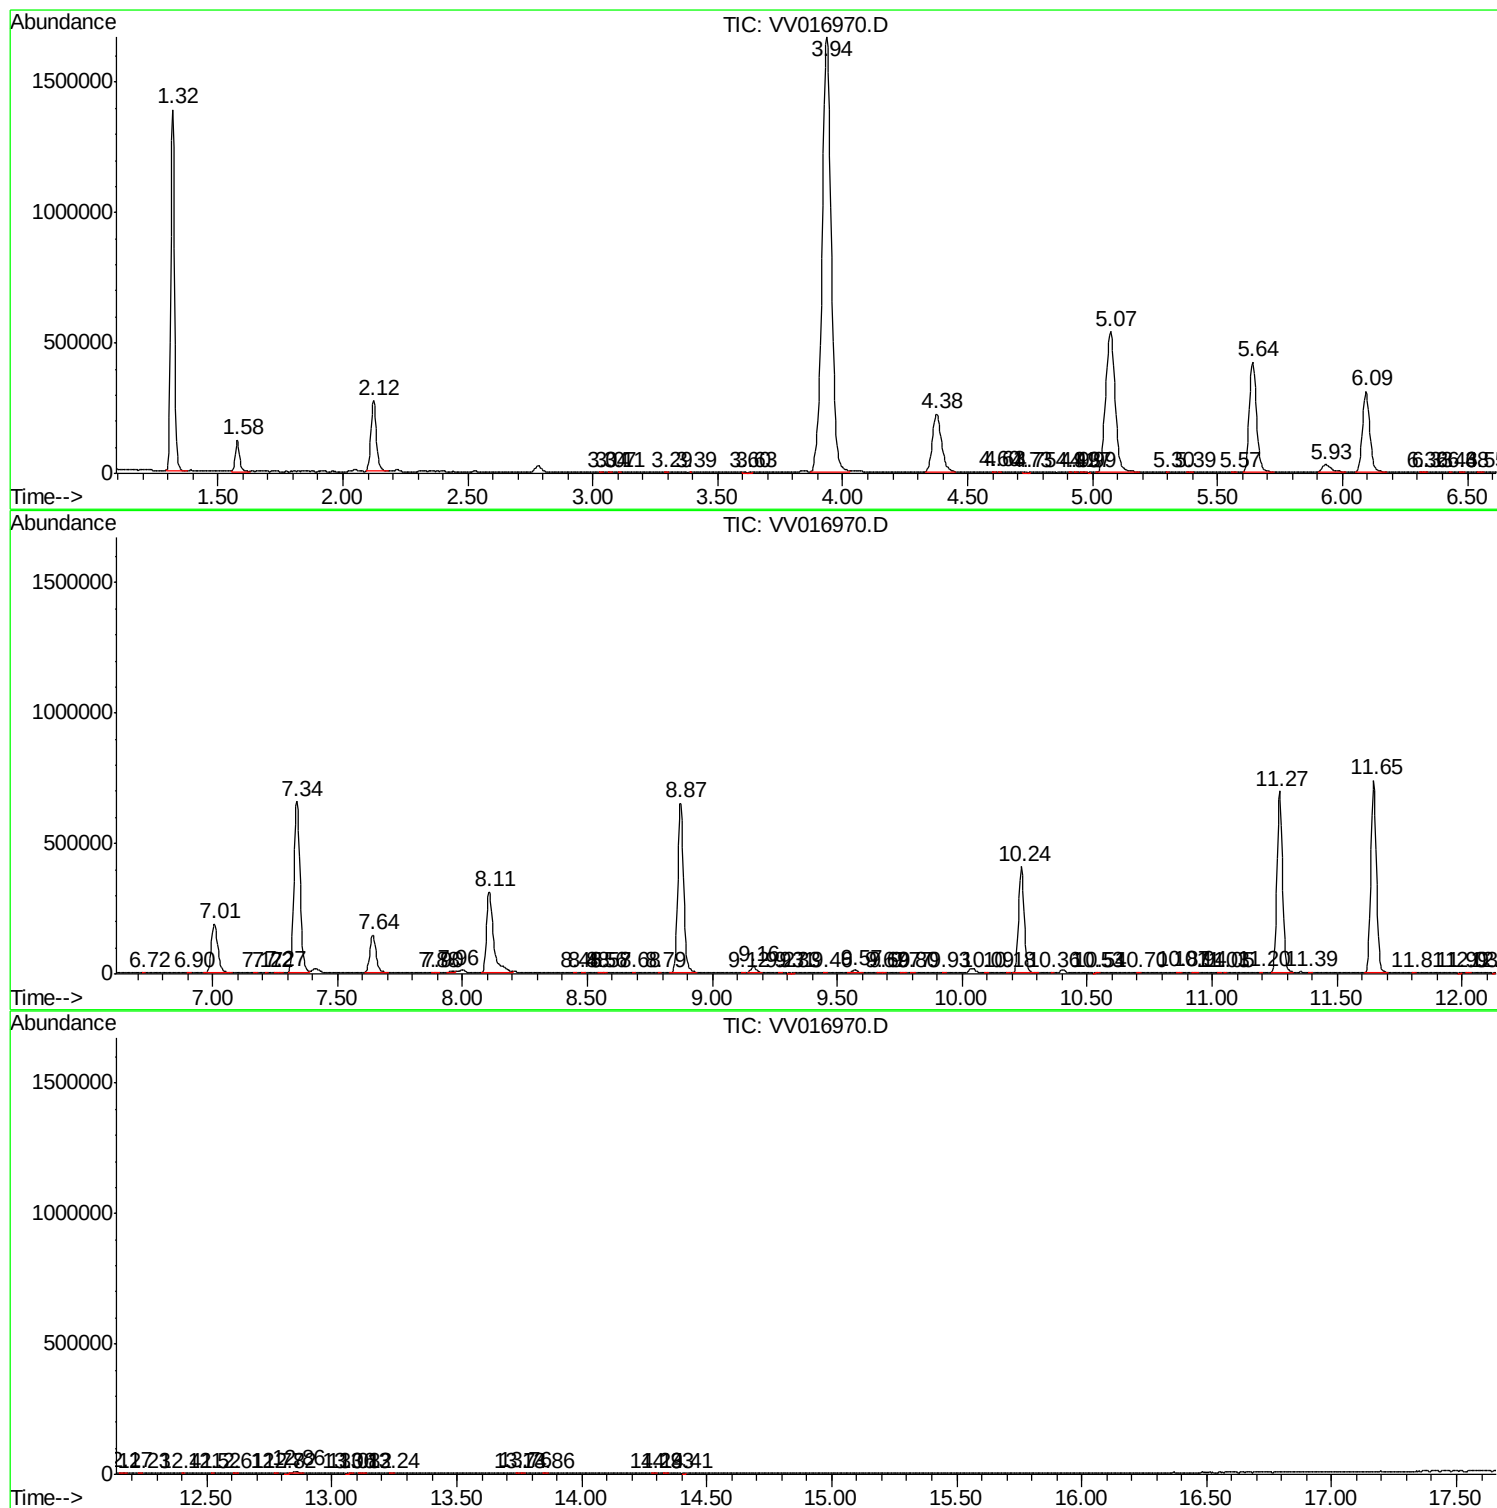

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016970.D
Acq On : 18 Jun 2020 11:41
Operator : SY/MD
Sample : L3039-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M00

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016970.D
Acq On : 18 Jun 2020 11:41
Operator : SY/MD
Sample : L3039-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M00

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc