

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016974.D
 Acq On : 18 Jun 2020 13:14
 Operator : SY/MD
 Sample : L3039-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	147194	150346	10.96%	1.346%
2	1.579	145	152	164	rVB	119722	132499	9.66%	1.186%
3	2.123	312	321	340	rBV	255941	388012	28.28%	3.473%
4	2.557	454	456	461	rBV4	1343	1104	0.08%	0.010%
5	2.759	517	519	520	rBV	1084	518	0.04%	0.005%
6	2.836	541	543	545	rBV2	1927	852	0.06%	0.008%
7	2.901	560	563	566	rBV5	1164	993	0.07%	0.009%
8	2.917	566	568	574	rVB6	1649	1198	0.09%	0.011%
9	2.962	580	582	586	rBV3	1369	957	0.07%	0.009%
10	3.004	593	595	599	rVB4	1571	782	0.06%	0.007%
11	3.036	603	605	608	rBV3	1349	645	0.05%	0.006%
12	3.106	625	627	629	rBV3	1962	1210	0.09%	0.011%
13	3.267	674	677	679	rBV4	1701	1131	0.08%	0.010%
14	3.389	712	715	719	rBV4	1919	1261	0.09%	0.011%
15	3.418	719	724	725	rBV4	1460	1068	0.08%	0.010%
16	3.447	731	733	737	rVB4	1897	894	0.07%	0.008%
17	3.521	754	756	759	rVB3	1268	517	0.04%	0.005%
18	3.537	759	761	766	rBV4	1119	840	0.06%	0.008%
19	3.566	768	770	773	rVB3	1470	716	0.05%	0.006%
20	3.618	782	786	788	rBV6	2047	1643	0.12%	0.015%
21	3.746	820	826	828	rBV4	1372	1308	0.10%	0.012%
22	3.817	846	848	850	rBV3	1236	733	0.05%	0.007%
23	3.913	866	878	911	rVV3	104270	413877	30.17%	3.704%
24	4.376	1009	1022	1048	rVB	213821	543997	39.65%	4.868%
25	4.521	1064	1067	1069	rBV3	1347	783	0.06%	0.007%
26	4.791	1147	1151	1152	rBV3	1467	721	0.05%	0.006%
27	4.965	1201	1205	1207	rBV4	1663	1013	0.07%	0.009%
28	5.074	1220	1239	1266	rBV2	522720	1371853	100.00%	12.277%
29	5.454	1355	1357	1359	rBV3	1146	564	0.04%	0.005%
30	5.466	1359	1361	1366	rVB5	1494	1204	0.09%	0.011%
31	5.643	1403	1416	1440	rVV	427459	847988	61.81%	7.589%
32	6.093	1544	1556	1576	rBV	304366	613448	44.72%	5.490%
33	6.383	1644	1646	1647	rBV2	1535	693	0.05%	0.006%
34	6.418	1656	1657	1662	rVB4	1810	1109	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016974.D
 Acq On : 18 Jun 2020 13:14
 Operator : SY/MD
 Sample : L3039-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.441	1662	1664	1665	rBV2	1333	492	0.04%	0.004%
36	6.569	1702	1704	1709	rVB4	1039	553	0.04%	0.005%
37	6.650	1726	1729	1730	rBV4	1342	664	0.05%	0.006%
38	6.765	1763	1765	1767	rVB2	2002	863	0.06%	0.008%
39	6.888	1800	1803	1806	rBV4	1400	1146	0.08%	0.010%
40	7.007	1829	1840	1854	rBV	182186	319607	23.30%	2.860%
41	7.154	1883	1886	1889	rBV4	1936	1687	0.12%	0.015%
42	7.338	1929	1943	1962	rBV	647867	1116076	81.36%	9.988%
43	7.643	2027	2038	2063	rVB	131075	229394	16.72%	2.053%
44	7.730	2063	2065	2068	rBV3	1798	1359	0.10%	0.012%
45	7.801	2084	2087	2091	rBV4	1420	1364	0.10%	0.012%
46	7.936	2127	2129	2130	rBV2	1506	603	0.04%	0.005%
47	7.997	2137	2148	2163	rVB	311502	514305	37.49%	4.603%
48	8.109	2173	2183	2210	rBV	318365	591545	43.12%	5.294%
49	8.363	2258	2262	2266	rBV7	1503	1281	0.09%	0.011%
50	8.746	2378	2381	2383	rBV4	1565	958	0.07%	0.009%
51	8.875	2408	2421	2443	rBV	652294	1051734	76.67%	9.412%
52	9.199	2520	2522	2524	rBV3	1325	593	0.04%	0.005%
53	9.232	2530	2532	2533	rBV2	1565	708	0.05%	0.006%
54	9.453	2598	2601	2605	rVB6	2047	1514	0.11%	0.014%
55	9.479	2607	2609	2614	rVV6	1593	1250	0.09%	0.011%
56	9.537	2625	2627	2628	rBV2	1158	466	0.03%	0.004%
57	9.617	2649	2652	2655	rVB4	1520	1016	0.07%	0.009%
58	9.685	2669	2673	2675	rBV4	1317	1032	0.08%	0.009%
59	9.730	2684	2687	2690	rVB3	1782	923	0.07%	0.008%
60	9.830	2715	2718	2719	rBV2	1203	492	0.04%	0.004%
61	9.887	2733	2736	2741	rBV6	821	743	0.05%	0.007%
62	9.997	2767	2770	2772	rBV4	1233	787	0.06%	0.007%
63	10.039	2781	2783	2785	rBV3	1398	677	0.05%	0.006%
64	10.061	2787	2790	2791	rBV3	1378	740	0.05%	0.007%
65	10.106	2797	2804	2805	rBV6	1553	1545	0.11%	0.014%
66	10.180	2822	2827	2831	rBV6	699	645	0.05%	0.006%
67	10.238	2833	2845	2860	rBV	388803	620595	45.24%	5.554%
68	10.444	2905	2909	2912	rVB4	2007	1849	0.13%	0.017%
69	10.466	2912	2916	2917	rBV4	922	689	0.05%	0.006%
70	10.675	2978	2981	2982	rBV3	1609	881	0.06%	0.008%
71	10.846	3031	3034	3035	rBV3	1553	964	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016974.D
 Acq On : 18 Jun 2020 13:14
 Operator : SY/MD
 Sample : L3039-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.932	3059	3061	3064	rBV4	1453	901	0.07%	0.008%
73	11.116	3112	3118	3121	rVB7	2101	2446	0.18%	0.022%
74	11.138	3121	3125	3128	rBV4	2042	1536	0.11%	0.014%
75	11.270	3155	3166	3183	rBV	702034	1070166	78.01%	9.577%
76	11.534	3246	3248	3250	rBV3	1274	601	0.04%	0.005%
77	11.646	3271	3283	3303	rBV	708270	1116773	81.41%	9.995%
78	11.923	3365	3369	3373	rBV6	1697	1312	0.10%	0.012%
79	11.942	3373	3375	3379	rVV2	1051	554	0.04%	0.005%
80	12.016	3394	3398	3403	rVV6	1122	1193	0.09%	0.011%
81	12.080	3415	3418	3419	rBV2	1016	492	0.04%	0.004%
82	12.158	3435	3442	3444	rBV6	1524	1698	0.12%	0.015%
83	12.228	3461	3464	3466	rBV4	1460	739	0.05%	0.007%
84	12.450	3530	3533	3536	rVB5	1562	1089	0.08%	0.010%
85	12.559	3565	3567	3570	rVB3	1535	884	0.06%	0.008%
86	12.585	3574	3575	3579	rVB4	798	444	0.03%	0.004%
87	12.611	3579	3583	3586	rBV5	1124	1188	0.09%	0.011%
88	12.765	3628	3631	3632	rBV2	1194	554	0.04%	0.005%
89	12.801	3640	3642	3644	rBV2	915	510	0.04%	0.005%
90	12.884	3661	3668	3671	rBV8	2156	3069	0.22%	0.027%
91	12.948	3685	3688	3691	rBV3	1077	620	0.05%	0.006%
92	13.148	3748	3750	3753	rBV3	1319	712	0.05%	0.006%
93	13.190	3759	3763	3767	rBV7	1694	1488	0.11%	0.013%
94	13.321	3801	3804	3805	rBV3	1400	766	0.06%	0.007%
95	13.868	3972	3974	3979	rVB5	1544	856	0.06%	0.008%
96	13.900	3982	3984	3988	rVB4	1614	720	0.05%	0.006%
97	13.977	4003	4008	4009	rBV4	1155	958	0.07%	0.009%
98	14.196	4071	4076	4078	rBV5	1758	1595	0.12%	0.014%
99	14.382	4130	4134	4136	rBV5	1344	1091	0.08%	0.010%
100	14.617	4205	4207	4209	rBV2	1680	674	0.05%	0.006%


Sum of corrected areas: 11173846

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016974.D
Acq On : 18 Jun 2020 13:14
Operator : SY/MD
Sample : L3039-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M08

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

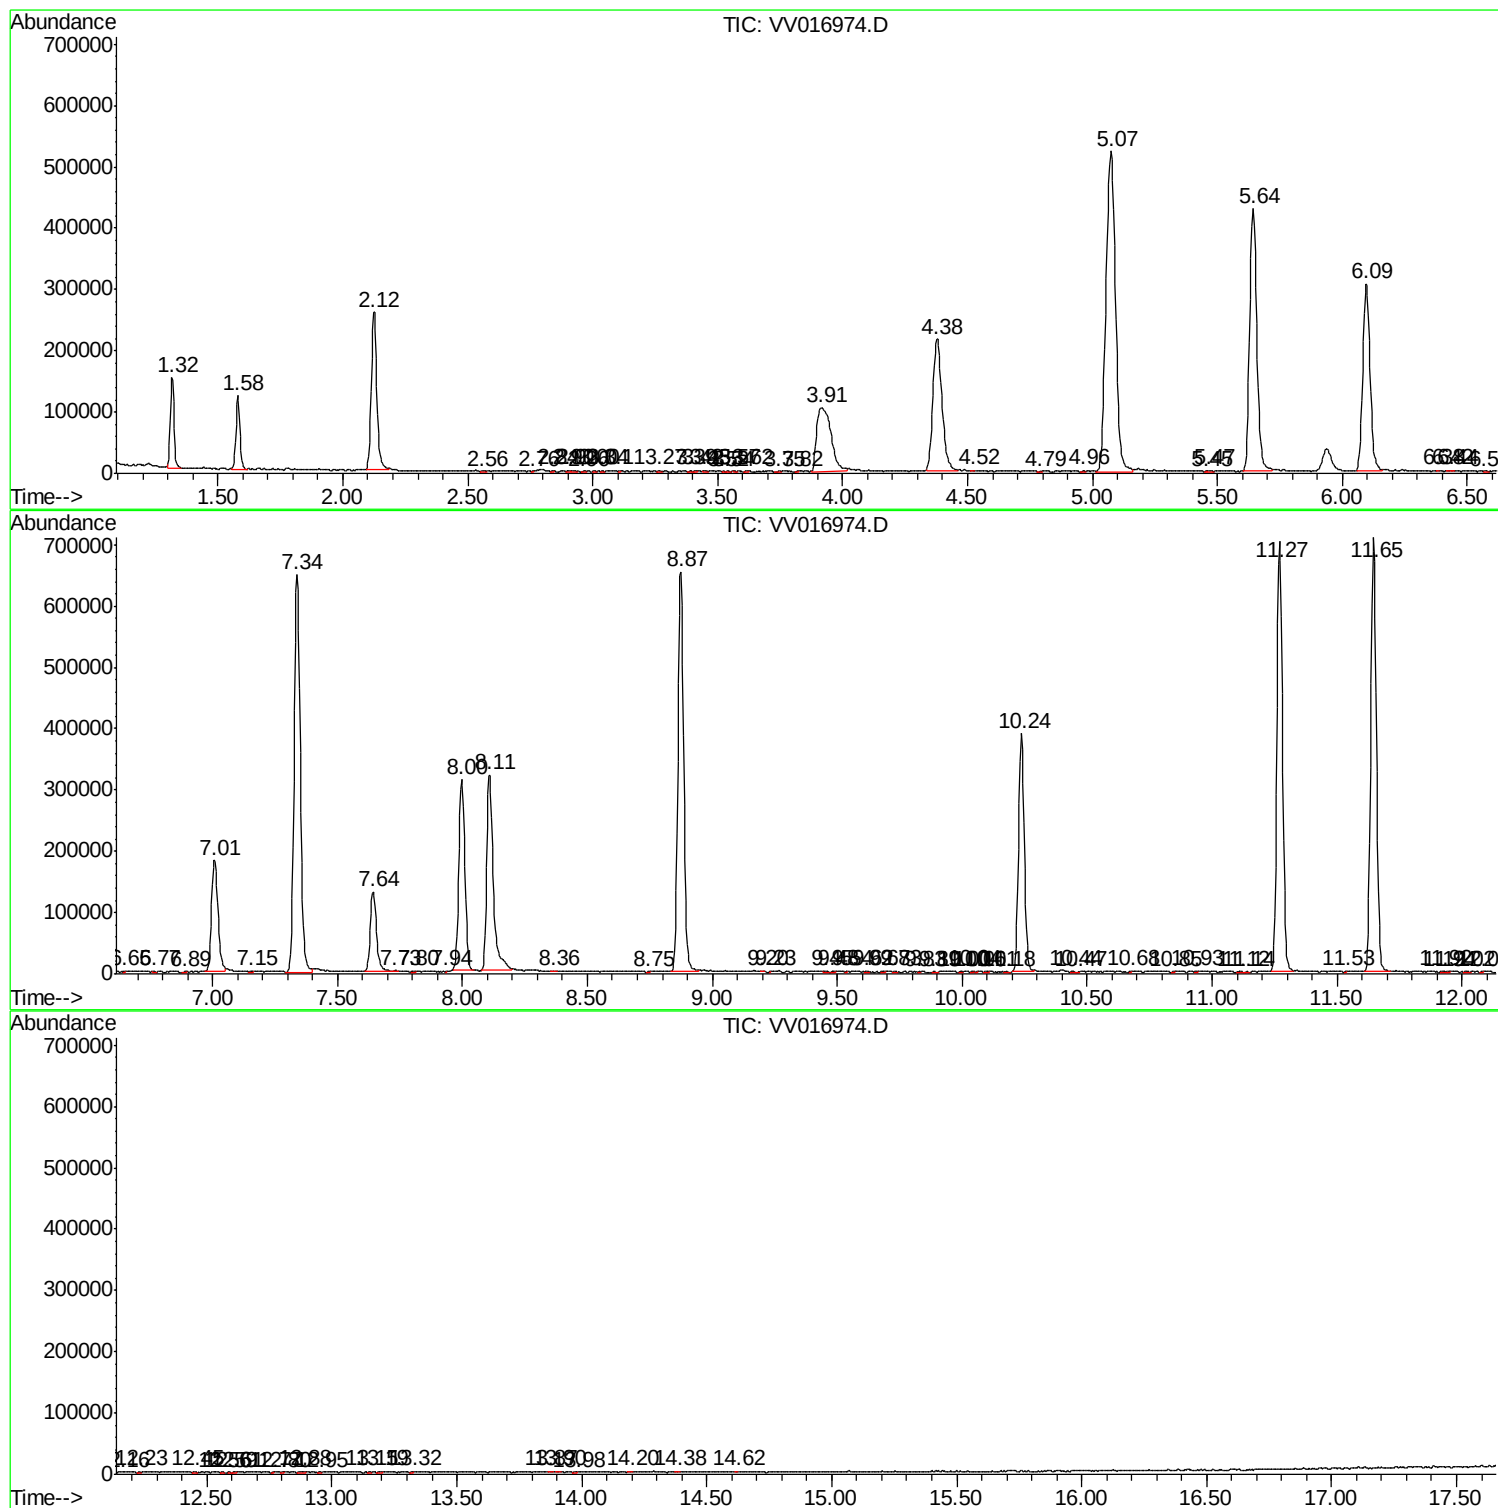

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016974.D
Acq On : 18 Jun 2020 13:14
Operator : SY/MD
Sample : L3039-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M08

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016974.D
Acq On : 18 Jun 2020 13:14
Operator : SY/MD
Sample : L3039-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M08

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc