

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016978.D
 Acq On : 18 Jun 2020 14:46
 Operator : SY/MD
 Sample : L3039-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	140855	149206	10.94%	1.476%
2	1.579	145	152	162	rBV	107388	120929	8.87%	1.196%
3	2.122	311	321	340	rBV	257535	388205	28.48%	3.841%
4	2.264	363	365	368	rBV3	1405	745	0.05%	0.007%
5	2.293	371	374	375	rBV3	1703	818	0.06%	0.008%
6	2.624	474	477	480	rBV5	1565	922	0.07%	0.009%
7	2.704	496	502	503	rBV5	1001	716	0.05%	0.007%
8	3.045	604	608	611	rBV5	1277	1063	0.08%	0.011%
9	3.103	623	626	630	rBV6	1692	1407	0.10%	0.014%
10	3.158	639	643	645	rBV3	2059	1410	0.10%	0.014%
11	3.238	665	668	670	rVB3	1460	736	0.05%	0.007%
12	3.261	670	675	678	rBV6	1376	1330	0.10%	0.013%
13	3.306	684	689	692	rVB7	1285	1042	0.08%	0.010%
14	3.389	712	715	718	rBV5	1294	1067	0.08%	0.011%
15	3.421	722	725	730	rVB6	1474	1280	0.09%	0.013%
16	3.463	734	738	740	rBV6	873	799	0.06%	0.008%
17	3.505	746	751	753	rBV4	1707	1229	0.09%	0.012%
18	3.598	775	780	784	rBV7	1717	1414	0.10%	0.014%
19	3.617	784	786	789	rVB3	1698	819	0.06%	0.008%
20	3.650	792	796	799	rBV4	1454	999	0.07%	0.010%
21	3.666	799	801	805	rBV5	1247	1081	0.08%	0.011%
22	3.688	805	808	813	rVB4	1137	851	0.06%	0.008%
23	3.830	846	852	856	rBV8	1499	1973	0.14%	0.020%
24	3.910	865	877	913	rBV	91829	277962	20.39%	2.750%
25	4.212	969	971	973	rBV3	1352	698	0.05%	0.007%
26	4.376	1002	1022	1046	rBV	239157	603339	44.26%	5.969%
27	4.679	1113	1116	1120	rBV6	2340	1451	0.11%	0.014%
28	4.730	1129	1132	1138	rVB7	2024	1714	0.13%	0.017%
29	4.984	1208	1211	1214	rVB4	1144	696	0.05%	0.007%
30	5.074	1221	1239	1265	rBV2	535933	1363293	100.00%	13.488%
31	5.415	1342	1345	1346	rBV2	1371	789	0.06%	0.008%
32	5.543	1383	1385	1388	rVB4	1415	682	0.05%	0.007%
33	5.592	1396	1400	1401	rBV3	1127	890	0.07%	0.009%
34	5.643	1403	1416	1437	rVV	380087	763230	55.98%	7.551%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016978.D
 Acq On : 18 Jun 2020 14:46
 Operator : SY/MD
 Sample : L3039-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.884	1487	1491	1492	rBV4	1425	797	0.06%	0.008%
36	5.929	1495	1505	1521	rVV2	39377	80144	5.88%	0.793%
37	6.093	1544	1556	1579	rVB	299939	609936	44.74%	6.035%
38	6.312	1620	1624	1627	rBV5	1599	1208	0.09%	0.012%
39	6.553	1697	1699	1700	rBV2	1395	728	0.05%	0.007%
40	6.576	1704	1706	1713	rVB8	1161	1215	0.09%	0.012%
41	6.604	1713	1715	1718	rBV4	1099	840	0.06%	0.008%
42	6.637	1723	1725	1727	rBV2	1770	1076	0.08%	0.011%
43	6.656	1729	1731	1735	rVB5	2071	1290	0.09%	0.013%
44	6.781	1767	1770	1772	rBV4	1551	1069	0.08%	0.011%
45	6.910	1807	1810	1813	rVB4	1782	844	0.06%	0.008%
46	7.010	1829	1841	1859	rBV	174772	313335	22.98%	3.100%
47	7.260	1917	1919	1921	rBV3	1414	729	0.05%	0.007%
48	7.338	1930	1943	1961	rBV	629430	1088062	79.81%	10.765%
49	7.643	2028	2038	2058	rBV	125671	212773	15.61%	2.105%
50	7.833	2094	2097	2098	rBV3	1620	960	0.07%	0.009%
51	8.032	2157	2159	2165	rVB7	1482	1355	0.10%	0.013%
52	8.109	2173	2183	2224	rBV2	281429	595116	43.65%	5.888%
53	8.530	2309	2314	2316	rBV4	1637	1338	0.10%	0.013%
54	8.688	2360	2363	2365	rBV3	1107	672	0.05%	0.007%
55	8.717	2369	2372	2375	rBV5	1366	948	0.07%	0.009%
56	8.733	2375	2377	2380	rBV3	848	650	0.05%	0.006%
57	8.874	2408	2421	2438	rBV	565941	922350	67.66%	9.125%
58	9.080	2482	2485	2489	rBV6	1474	1346	0.10%	0.013%
59	9.157	2503	2509	2510	rBV4	2828	2559	0.19%	0.025%
60	9.222	2527	2529	2531	rBV3	1496	807	0.06%	0.008%
61	9.257	2535	2540	2542	rBV4	1511	1002	0.07%	0.010%
62	9.405	2583	2586	2588	rBV3	1561	853	0.06%	0.008%
63	9.463	2600	2604	2607	rVB6	1466	1250	0.09%	0.012%
64	9.505	2613	2617	2620	rBV6	1228	935	0.07%	0.009%
65	9.575	2634	2639	2651	rVV6	7974	15865	1.16%	0.157%
66	9.743	2687	2691	2693	rBV4	2082	1399	0.10%	0.014%
67	9.775	2697	2701	2707	rVV7	1932	1744	0.13%	0.017%
68	9.887	2733	2736	2738	rBV4	1425	806	0.06%	0.008%
69	9.981	2760	2765	2769	rBV5	2132	1811	0.13%	0.018%
70	10.038	2779	2783	2787	rBV7	1370	1165	0.09%	0.012%
71	10.148	2811	2817	2821	rBV7	1903	1342	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016978.D
 Acq On : 18 Jun 2020 14:46
 Operator : SY/MD
 Sample : L3039-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.238	2833	2845	2862	rBV	359426	558370	40.96%	5.524%
73	10.370	2882	2886	2889	rBV4	1525	1191	0.09%	0.012%
74	10.878	3038	3044	3046	rBV6	2957	2743	0.20%	0.027%
75	10.923	3054	3058	3060	rBV3	1506	953	0.07%	0.009%
76	10.942	3061	3064	3070	rVV8	1789	1892	0.14%	0.019%
77	11.054	3095	3099	3104	rBV8	1158	1182	0.09%	0.012%
78	11.154	3125	3130	3132	rBV6	1905	1848	0.14%	0.018%
79	11.270	3155	3166	3187	rVB	582477	897534	65.84%	8.880%
80	11.440	3215	3219	3221	rBV4	1467	1133	0.08%	0.011%
81	11.646	3272	3283	3303	rVB	679821	1049713	77.00%	10.386%
82	11.775	3321	3323	3325	rBV3	1877	801	0.06%	0.008%
83	11.900	3359	3362	3365	rVB3	1259	804	0.06%	0.008%
84	11.926	3365	3370	3373	rBV5	1867	1931	0.14%	0.019%
85	12.070	3413	3415	3417	rBV2	1892	957	0.07%	0.009%
86	12.099	3422	3424	3430	rBV6	1305	1260	0.09%	0.012%
87	12.228	3462	3464	3468	rVB5	1102	654	0.05%	0.006%
88	12.267	3468	3476	3477	rBV7	2468	2759	0.20%	0.027%
89	12.325	3490	3494	3498	rBV7	2511	1904	0.14%	0.019%
90	13.090	3729	3732	3736	rBV5	1829	1529	0.11%	0.015%
91	13.492	3854	3857	3861	rBV	4389	2724	0.20%	0.027%
92	13.604	3888	3892	3895	rVB4	2348	1665	0.12%	0.016%
93	13.865	3970	3973	3977	rBV5	1438	1253	0.09%	0.012%
94	13.977	4004	4008	4010	rVV5	1096	834	0.06%	0.008%
95	14.086	4040	4042	4044	rBV3	1250	657	0.05%	0.007%
96	14.154	4061	4063	4066	rVB4	1415	726	0.05%	0.007%
97	14.186	4066	4073	4074	rBV5	2008	1949	0.14%	0.019%
98	14.820	4267	4270	4272	rBV3	2064	1154	0.08%	0.011%
99	14.877	4285	4288	4291	rBV4	1307	1051	0.08%	0.010%
100	15.385	4442	4446	4447	rBV5	1639	1161	0.09%	0.011%


Sum of corrected areas: 10107436

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016978.D
Acq On : 18 Jun 2020 14:46
Operator : SY/MD
Sample : L3039-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

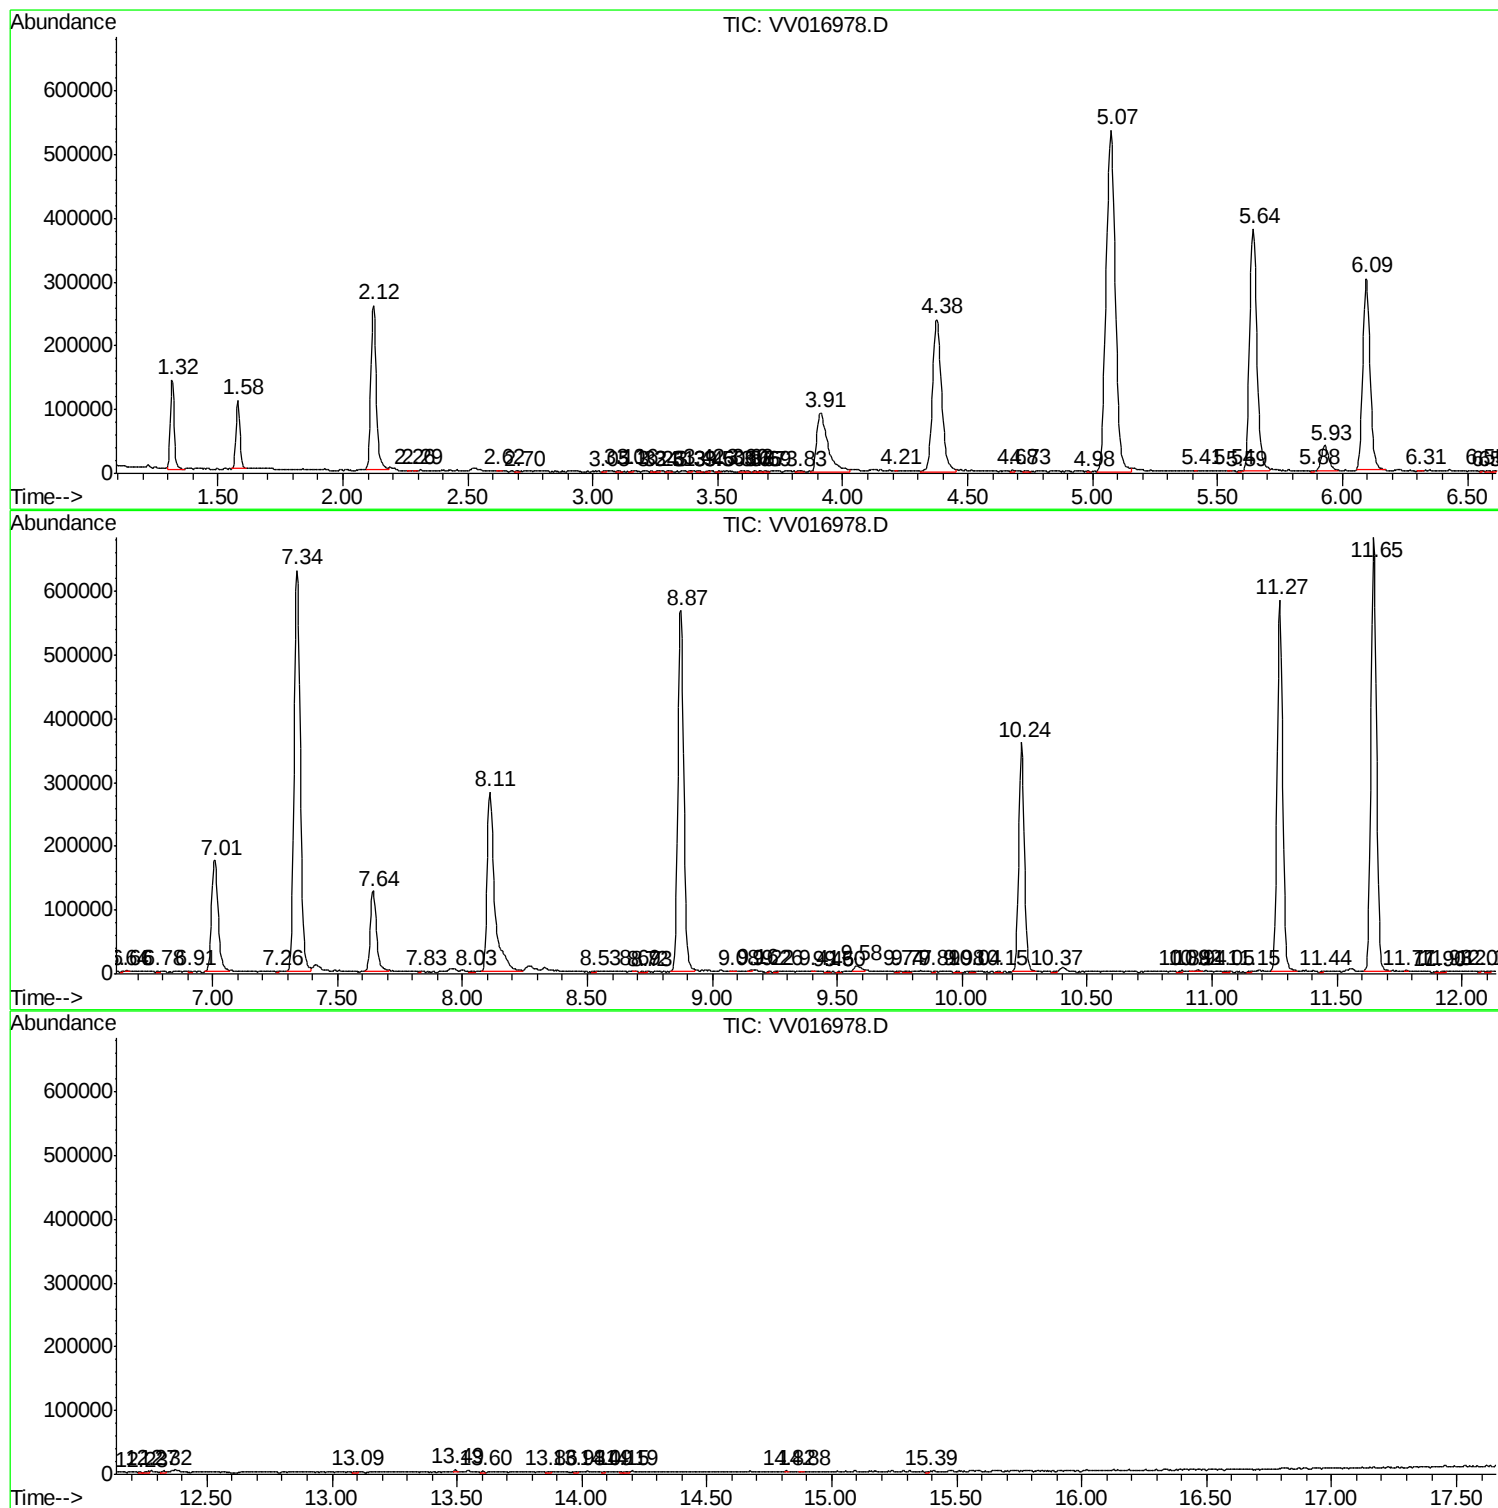

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016978.D
Acq On : 18 Jun 2020 14:46
Operator : SY/MD
Sample : L3039-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016978.D
Acq On : 18 Jun 2020 14:46
Operator : SY/MD
Sample : L3039-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M22

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc