

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016979.D
 Acq On : 18 Jun 2020 15:09
 Operator : SY/MD
 Sample : L3039-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	141435	145659	9.18%	1.210%
2	1.579	144	152	162	rBV	113087	127115	8.01%	1.056%
3	2.123	311	321	340	rBV	256136	376708	23.74%	3.130%
4	2.505	436	440	441	rBV3	1213	765	0.05%	0.006%
5	2.962	580	582	585	rBV3	1183	557	0.04%	0.005%
6	2.984	585	589	590	rBV4	833	503	0.03%	0.004%
7	3.045	605	608	610	rBV3	1539	719	0.05%	0.006%
8	3.190	651	653	656	rVB3	1397	563	0.04%	0.005%
9	3.209	656	659	661	rBV4	1303	752	0.05%	0.006%
10	3.303	685	688	691	rBV4	991	651	0.04%	0.005%
11	3.341	698	700	704	rBV5	947	621	0.04%	0.005%
12	3.418	719	724	727	rBV6	1826	1898	0.12%	0.016%
13	3.505	748	751	752	rVV2	1471	819	0.05%	0.007%
14	3.528	756	758	761	rVB2	789	473	0.03%	0.004%
15	3.553	764	766	769	rVB3	1501	647	0.04%	0.005%
16	3.621	783	787	792	rVV7	1827	1959	0.12%	0.016%
17	3.643	792	794	795	rVV2	1474	488	0.03%	0.004%
18	3.676	802	804	809	rVB3	2041	1138	0.07%	0.009%
19	3.708	809	814	816	rBV5	1476	1226	0.08%	0.010%
20	3.737	821	823	827	rBV5	1119	857	0.05%	0.007%
21	3.923	867	881	904	rBV2	109349	412188	25.98%	3.425%
22	4.274	987	990	991	rBV2	1218	743	0.05%	0.006%
23	4.376	1005	1022	1046	rBV	215411	545169	34.36%	4.529%
24	5.074	1221	1239	1267	rBV2	517653	1338577	84.36%	11.121%
25	5.319	1313	1315	1318	rBV4	1737	903	0.06%	0.008%
26	5.454	1355	1357	1360	rBV4	1120	709	0.04%	0.006%
27	5.640	1403	1415	1433	rBV	422463	843674	53.17%	7.009%
28	5.939	1497	1508	1524	rVB4	68660	145633	9.18%	1.210%
29	6.093	1541	1556	1579	rBV	299957	613317	38.65%	5.096%
30	6.338	1630	1632	1634	rBV2	1646	743	0.05%	0.006%
31	6.383	1642	1646	1648	rBV4	1430	1350	0.09%	0.011%
32	6.566	1700	1703	1706	rVB4	1252	760	0.05%	0.006%
33	6.582	1706	1708	1709	rBV2	1271	554	0.03%	0.005%
34	6.849	1788	1791	1792	rBV3	1075	554	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016979.D
 Acq On : 18 Jun 2020 15:09
 Operator : SY/MD
 Sample : L3039-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.859	1792	1794	1796	rVV3	1473	628	0.04%	0.005%
36	6.891	1802	1804	1806	rBV3	1494	944	0.06%	0.008%
37	6.936	1814	1818	1819	rBV3	1098	680	0.04%	0.006%
38	6.955	1821	1824	1829	rVV6	1513	1605	0.10%	0.013%
39	7.007	1830	1840	1856	rVV	170336	305047	19.22%	2.534%
40	7.187	1894	1896	1897	rBV2	1518	679	0.04%	0.006%
41	7.293	1927	1929	1931	rBV3	1458	666	0.04%	0.006%
42	7.338	1931	1943	1962	rVV	623674	1075215	67.76%	8.933%
43	7.643	2023	2038	2059	rBV	124153	222224	14.01%	1.846%
44	7.997	2137	2148	2164	rVB	952082	1586723	100.00%	13.183%
45	8.109	2173	2183	2213	rBV	307408	587672	37.04%	4.883%
46	8.598	2333	2335	2338	rBV3	1093	725	0.05%	0.006%
47	8.640	2346	2348	2350	rBV	1534	828	0.05%	0.007%
48	8.781	2388	2392	2394	rBV4	1529	1398	0.09%	0.012%
49	8.875	2407	2421	2444	rBV	645287	1038206	65.43%	8.626%
50	9.068	2478	2481	2482	rBV2	1383	761	0.05%	0.006%
51	9.161	2508	2510	2515	rBV5	1575	1395	0.09%	0.012%
52	9.225	2528	2530	2532	rBV2	1263	693	0.04%	0.006%
53	9.244	2534	2536	2539	rBV5	1318	589	0.04%	0.005%
54	9.408	2586	2587	2590	rBV3	1073	605	0.04%	0.005%
55	9.489	2610	2612	2616	rBV5	1321	758	0.05%	0.006%
56	9.611	2645	2650	2653	rBV7	1393	1278	0.08%	0.011%
57	9.669	2666	2668	2671	rVB5	1433	604	0.04%	0.005%
58	9.691	2671	2675	2676	rBV3	1153	761	0.05%	0.006%
59	9.762	2695	2697	2699	rBV3	1285	694	0.04%	0.006%
60	9.778	2699	2702	2705	rVV4	1221	869	0.05%	0.007%
61	10.006	2770	2773	2774	rBV3	1158	563	0.04%	0.005%
62	10.026	2778	2779	2785	rVB6	1308	1028	0.06%	0.009%
63	10.064	2788	2791	2793	rBV4	1091	813	0.05%	0.007%
64	10.116	2805	2807	2811	rVB5	2007	1061	0.07%	0.009%
65	10.132	2811	2812	2817	rVB4	1497	1100	0.07%	0.009%
66	10.167	2817	2823	2827	rBV8	2725	2528	0.16%	0.021%
67	10.238	2832	2845	2862	rBV	382330	594136	37.44%	4.936%
68	10.868	3038	3041	3043	rBV3	1575	1067	0.07%	0.009%
69	10.971	3071	3073	3075	rBV2	1539	946	0.06%	0.008%
70	11.029	3087	3091	3093	rBV4	1723	1546	0.10%	0.013%
71	11.270	3154	3166	3184	rBV	649124	981988	61.89%	8.159%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016979.D
 Acq On : 18 Jun 2020 15:09
 Operator : SY/MD
 Sample : L3039-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M15

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.399	3204	3206	3207	rBV2	1227	470	0.03%	0.004%
73	11.646	3271	3283	3299	rBV	659659	1023928	64.53%	8.507%
74	11.833	3338	3341	3342	rBV3	1167	707	0.04%	0.006%
75	11.920	3364	3368	3370	rBV4	1520	1029	0.06%	0.009%
76	12.003	3392	3394	3396	rBV3	1372	693	0.04%	0.006%
77	12.090	3418	3421	3423	rBV4	1322	921	0.06%	0.008%
78	12.119	3427	3430	3431	rBV3	1082	472	0.03%	0.004%
79	12.241	3463	3468	3469	rBV3	1106	821	0.05%	0.007%
80	12.376	3508	3510	3512	rBV3	1560	508	0.03%	0.004%
81	12.415	3520	3522	3526	rBV3	998	699	0.04%	0.006%
82	12.595	3575	3578	3582	rBV5	1294	1140	0.07%	0.009%
83	12.656	3595	3597	3599	rBV3	1237	671	0.04%	0.006%
84	12.752	3623	3627	3629	rVV3	1067	802	0.05%	0.007%
85	12.858	3659	3660	3663	rBV2	825	548	0.03%	0.005%
86	12.916	3675	3678	3681	rVB2	1578	928	0.06%	0.008%
87	12.932	3681	3683	3686	rBV3	1244	932	0.06%	0.008%
88	12.974	3693	3696	3699	rBV4	1490	1024	0.06%	0.009%
89	13.032	3710	3714	3718	rBV6	1158	1049	0.07%	0.009%
90	13.395	3825	3827	3831	rVB4	1018	721	0.05%	0.006%
91	13.833	3961	3963	3966	rBV4	988	607	0.04%	0.005%
92	13.907	3984	3986	3991	rVB5	1639	1342	0.08%	0.011%
93	13.939	3994	3996	3998	rVV2	1132	549	0.03%	0.005%
94	13.961	4001	4003	4005	rBV3	1476	762	0.05%	0.006%
95	14.029	4022	4024	4026	rBV3	1312	555	0.03%	0.005%
96	14.193	4073	4075	4079	rBV5	1144	832	0.05%	0.007%
97	14.415	4141	4144	4145	rBV4	1498	753	0.05%	0.006%
98	14.720	4236	4239	4241	rBV4	1495	1121	0.07%	0.009%
99	14.987	4319	4322	4327	rBV6	2255	2630	0.17%	0.022%
100	15.235	4397	4399	4401	rBV3	1772	934	0.06%	0.008%


Sum of corrected areas: 12036163

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016979.D
Acq On : 18 Jun 2020 15:09
Operator : SY/MD
Sample : L3039-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M15

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

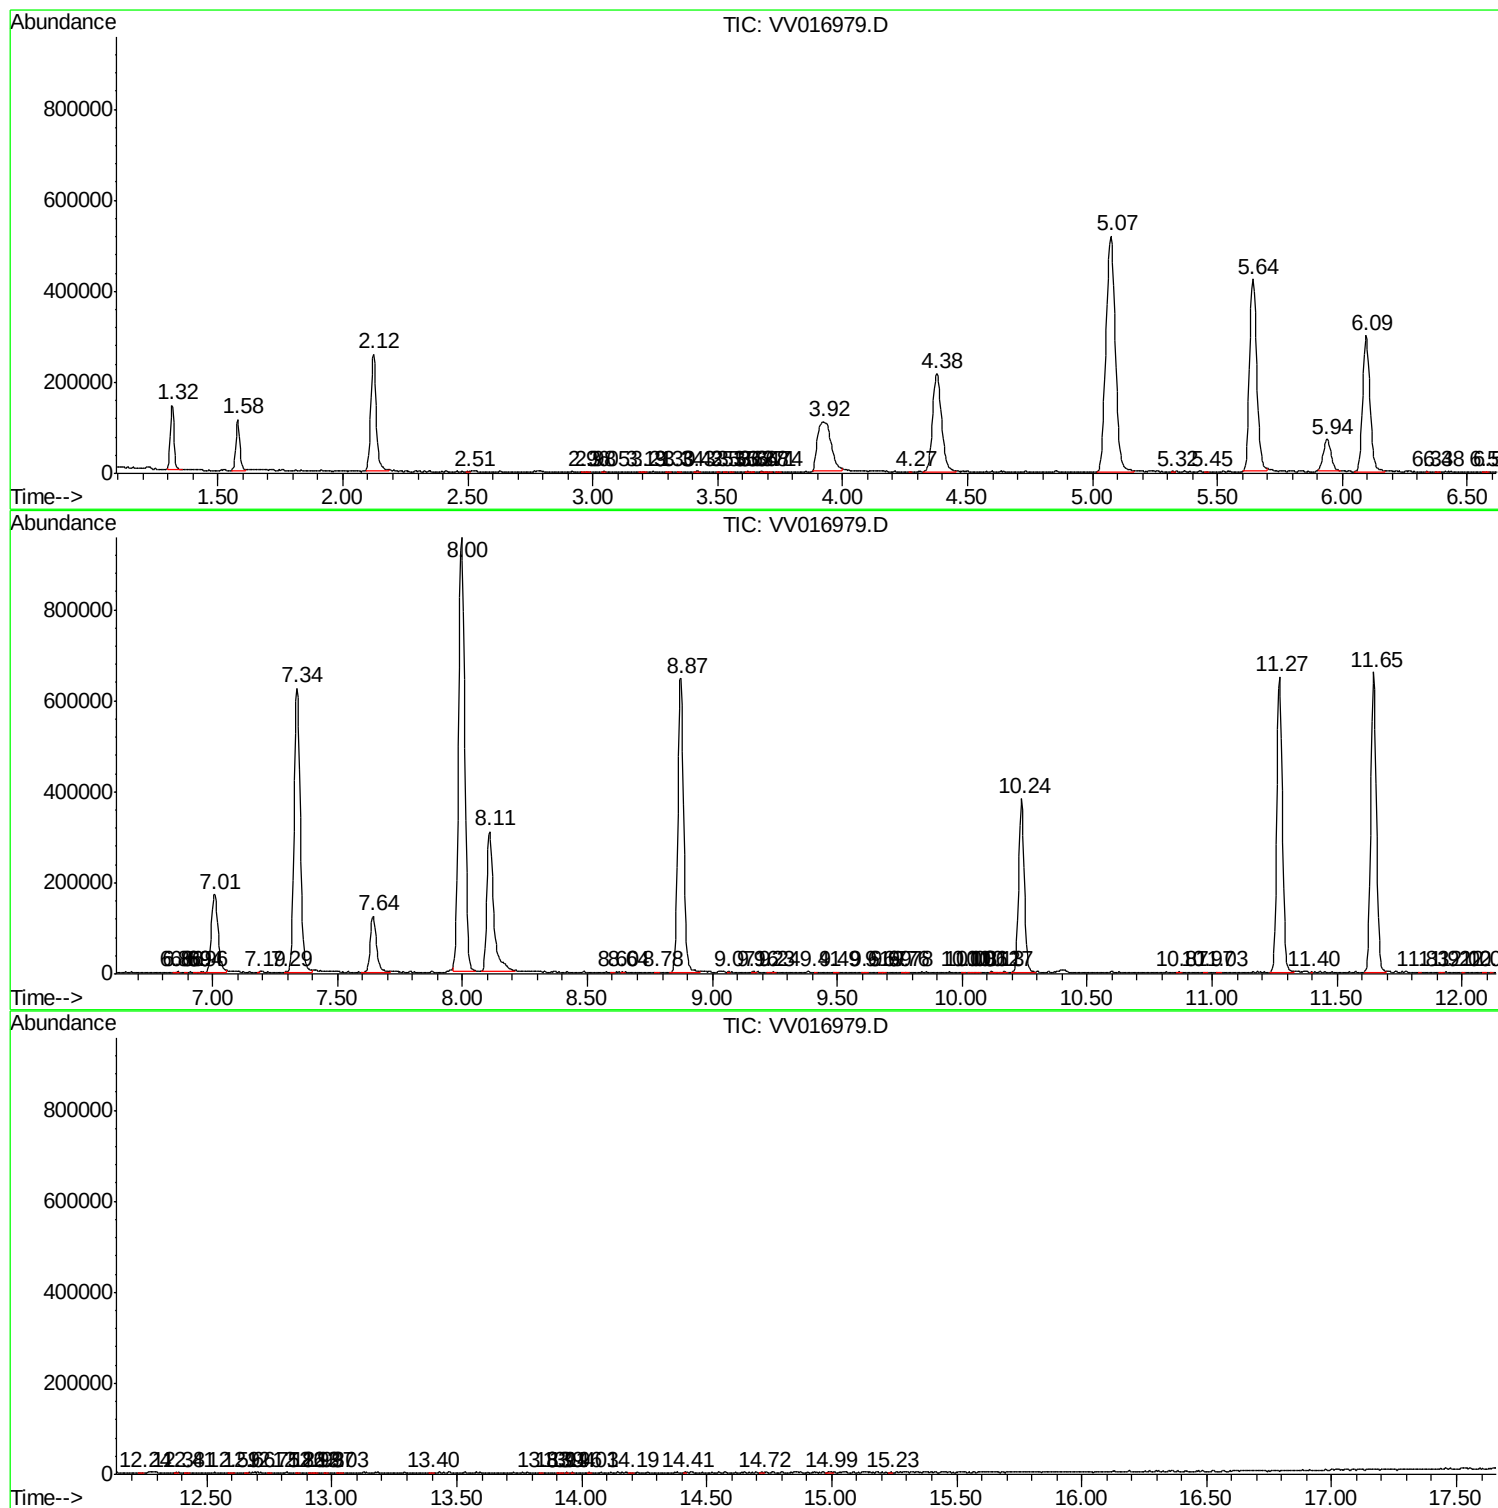

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016979.D
Acq On : 18 Jun 2020 15:09
Operator : SY/MD
Sample : L3039-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M15

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016979.D
Acq On : 18 Jun 2020 15:09
Operator : SY/MD
Sample : L3039-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M15

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc