

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016981.D
 Acq On : 18 Jun 2020 15:56
 Operator : SY/MD
 Sample : L3039-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	107082	109410	10.36%	1.309%
2	1.579	145	152	161	rBV	81353	88897	8.42%	1.064%
3	2.123	312	321	337	rBV	191568	286756	27.16%	3.431%
4	2.688	493	497	503	rBV6	1569	1464	0.14%	0.018%
5	3.004	589	595	598	rBV8	1533	1354	0.13%	0.016%
6	3.049	603	609	615	rBV8	2528	3572	0.34%	0.043%
7	3.087	616	621	624	rVB5	1490	1296	0.12%	0.016%
8	3.274	677	679	684	rBV5	932	795	0.08%	0.010%
9	3.444	730	732	736	rVB4	1494	969	0.09%	0.012%
10	3.473	737	741	743	rBV5	1043	795	0.08%	0.010%
11	3.528	754	758	762	rBV6	1899	1532	0.15%	0.018%
12	3.579	773	774	777	rVB3	1758	706	0.07%	0.008%
13	3.602	777	781	785	rBV7	1566	1343	0.13%	0.016%
14	3.624	785	788	792	rVV5	1780	1042	0.10%	0.012%
15	3.672	798	803	806	rBV5	1769	1463	0.14%	0.018%
16	3.711	812	815	817	rBV4	1685	943	0.09%	0.011%
17	3.750	823	827	829	rBV3	1488	1024	0.10%	0.012%
18	3.811	843	846	850	rBV5	1459	1141	0.11%	0.014%
19	3.836	850	854	856	rBV4	939	748	0.07%	0.009%
20	3.910	866	877	913	rBV	89951	293263	27.77%	3.509%
21	4.158	951	954	956	rBV4	1570	1138	0.11%	0.014%
22	4.377	1009	1022	1046	rVB	173981	422409	40.01%	5.055%
23	4.901	1182	1185	1187	rBV3	1447	919	0.09%	0.011%
24	4.926	1190	1193	1195	rBV4	1116	709	0.07%	0.008%
25	5.071	1218	1238	1265	rBV3	404986	1055864	100.00%	12.635%
26	5.248	1291	1293	1301	rVB9	1924	2149	0.20%	0.026%
27	5.335	1318	1320	1324	rBV4	1222	835	0.08%	0.010%
28	5.579	1394	1396	1402	rVB6	1463	1156	0.11%	0.014%
29	5.640	1402	1415	1435	rBV	323184	649427	61.51%	7.771%
30	5.888	1487	1492	1494	rBV6	2180	1649	0.16%	0.020%
31	5.933	1494	1506	1522	rVB8	28555	67058	6.35%	0.802%
32	6.023	1532	1534	1537	rBV3	1925	1145	0.11%	0.014%
33	6.093	1544	1556	1578	rBV	239568	481435	45.60%	5.761%
34	6.450	1662	1667	1669	rBV5	1031	934	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016981.D
 Acq On : 18 Jun 2020 15:56
 Operator : SY/MD
 Sample : L3039-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.653	1725	1730	1734	rBV7	1925	2290	0.22%	0.027%
36	6.708	1745	1747	1751	rBV4	1022	695	0.07%	0.008%
37	6.727	1751	1753	1756	rVB3	1422	698	0.07%	0.008%
38	6.917	1809	1812	1815	rVB4	1420	1023	0.10%	0.012%
39	6.939	1817	1819	1823	rBV5	1154	895	0.08%	0.011%
40	7.010	1827	1841	1857	rBV	132265	241660	22.89%	2.892%
41	7.203	1898	1901	1905	rBV6	1134	995	0.09%	0.012%
42	7.338	1931	1943	1961	rBV	475241	824663	78.10%	9.868%
43	7.608	2023	2027	2028	rBV4	1463	1081	0.10%	0.013%
44	7.643	2028	2038	2058	rVV2	96512	169503	16.05%	2.028%
45	7.791	2082	2084	2088	rBV2	1586	950	0.09%	0.011%
46	7.846	2099	2101	2105	rVB5	1584	833	0.08%	0.010%
47	7.868	2106	2108	2111	rVB4	1100	651	0.06%	0.008%
48	7.894	2111	2116	2118	rBV4	1451	1129	0.11%	0.014%
49	7.997	2140	2148	2160	rVB	149266	244135	23.12%	2.921%
50	8.110	2173	2183	2218	rBV2	270492	533806	50.56%	6.388%
51	8.409	2274	2276	2282	rVB7	1530	861	0.08%	0.010%
52	8.544	2313	2318	2320	rBV6	1658	1515	0.14%	0.018%
53	8.585	2329	2331	2334	rVB3	1484	677	0.06%	0.008%
54	8.875	2409	2421	2443	rVV	475958	785657	74.41%	9.401%
55	9.019	2463	2466	2470	rBV5	2027	1401	0.13%	0.017%
56	9.151	2502	2507	2510	rBV6	2632	2876	0.27%	0.034%
57	9.360	2566	2572	2573	rBV5	1746	1224	0.12%	0.015%
58	9.386	2577	2580	2582	rBV3	1748	1218	0.12%	0.015%
59	9.444	2596	2598	2602	rBV3	1405	1003	0.09%	0.012%
60	9.691	2668	2675	2679	rBV8	1442	2159	0.20%	0.026%
61	9.910	2738	2743	2747	rBV6	1586	1675	0.16%	0.020%
62	9.990	2763	2768	2774	rBV10	1583	1441	0.14%	0.017%
63	10.029	2774	2780	2781	rBV4	1772	1446	0.14%	0.017%
64	10.061	2786	2790	2792	rBV5	987	805	0.08%	0.010%
65	10.164	2818	2822	2825	rVB5	1614	1249	0.12%	0.015%
66	10.238	2834	2845	2860	rBV	315592	494289	46.81%	5.915%
67	10.367	2882	2885	2888	rVB5	1445	892	0.08%	0.011%
68	10.402	2888	2896	2905	rBV7	5847	9948	0.94%	0.119%
69	10.592	2953	2955	2956	rBV2	1266	713	0.07%	0.009%
70	10.756	3003	3006	3007	rBV3	1594	980	0.09%	0.012%
71	10.826	3026	3028	3032	rBV3	1334	1051	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016981.D
 Acq On : 18 Jun 2020 15:56
 Operator : SY/MD
 Sample : L3039-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.029	3088	3091	3094	rBV4	1553	885	0.08%	0.011%
73	11.080	3104	3107	3109	rBV4	1522	1075	0.10%	0.013%
74	11.270	3155	3166	3183	rBV	467192	709184	67.17%	8.486%
75	11.469	3225	3228	3231	rBV5	1342	1033	0.10%	0.012%
76	11.646	3271	3283	3298	rBV	499078	790776	74.89%	9.463%
77	11.826	3336	3339	3343	rBV3	911	711	0.07%	0.009%
78	12.096	3421	3423	3427	rBV4	1277	1034	0.10%	0.012%
79	12.299	3484	3486	3489	rVB3	1601	733	0.07%	0.009%
80	12.370	3504	3508	3512	rBV7	2201	2721	0.26%	0.033%
81	12.669	3597	3601	3605	rBV6	1343	1402	0.13%	0.017%
82	12.714	3612	3615	3617	rBV5	1535	815	0.08%	0.010%
83	13.100	3733	3735	3739	rBV5	944	657	0.06%	0.008%
84	13.177	3756	3759	3762	rBV5	1877	1505	0.14%	0.018%
85	13.350	3810	3813	3818	rBV6	1744	1323	0.13%	0.016%
86	13.502	3858	3860	3865	rBV6	1298	1285	0.12%	0.015%
87	13.604	3886	3892	3895	rBV7	1733	2092	0.20%	0.025%
88	13.617	3895	3896	3903	rVB6	1889	1389	0.13%	0.017%
89	13.762	3938	3941	3943	rBV3	1327	796	0.08%	0.010%
90	14.167	4062	4067	4069	rBV3	1862	1343	0.13%	0.016%
91	14.186	4071	4073	4076	rVB3	1523	715	0.07%	0.009%
92	14.273	4097	4100	4102	rBV2	1645	890	0.08%	0.011%
93	14.370	4127	4130	4135	rVB7	1929	1551	0.15%	0.019%
94	14.392	4135	4137	4142	rBV6	1455	1457	0.14%	0.017%
95	14.530	4175	4180	4181	rBV4	1918	1595	0.15%	0.019%
96	14.878	4286	4288	4292	rVB3	1583	883	0.08%	0.011%
97	15.064	4343	4346	4349	rBV4	1993	1514	0.14%	0.018%
98	15.116	4359	4362	4365	rBV5	2125	1526	0.14%	0.018%
99	15.376	4441	4443	4445	rBV3	1471	806	0.08%	0.010%
100	15.505	4480	4483	4485	rBV3	2186	1601	0.15%	0.019%


Sum of corrected areas: 8356724

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016981.D
Acq On : 18 Jun 2020 15:56
Operator : SY/MD
Sample : L3039-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9M18

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

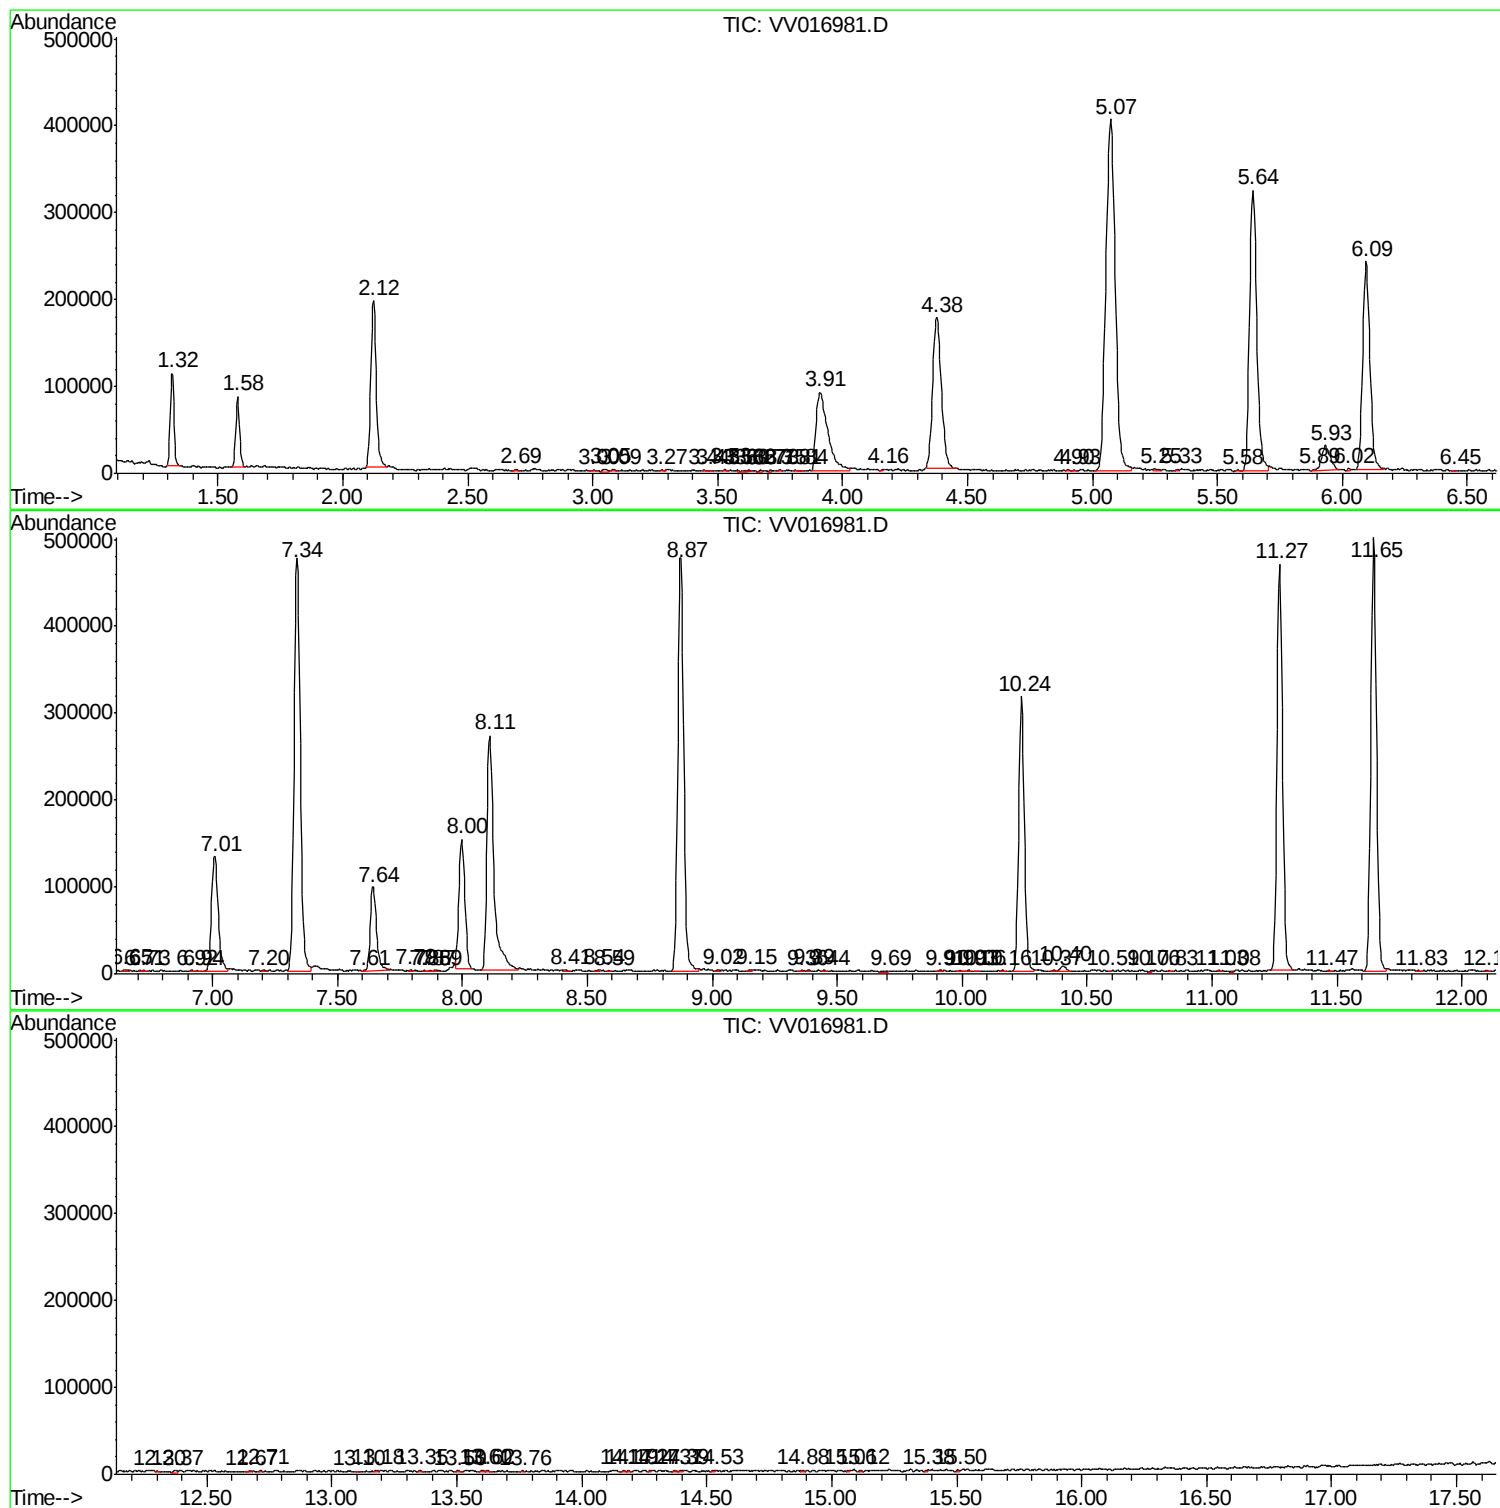

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016981.D
Acq On : 18 Jun 2020 15:56
Operator : SY/MD
Sample : L3039-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M18

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016981.D
Acq On : 18 Jun 2020 15:56
Operator : SY/MD
Sample : L3039-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M18

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc