

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016982.D
 Acq On : 18 Jun 2020 17:05
 Operator : SY/MD
 Sample : L3039-01DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M00DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.318	64	71	83	rVB2	248286	260467	19.38%	2.424%
2	1.579	146	152	162	rVB	105859	118252	8.80%	1.101%
3	2.122	311	321	341	rBV	254312	385234	28.67%	3.586%
4	2.351	390	392	394	rBV3	1431	508	0.04%	0.005%
5	2.466	425	428	434	rBV6	1371	1260	0.09%	0.012%
6	2.527	438	447	460	rVB4	8525	16493	1.23%	0.154%
7	2.614	472	474	476	rBV3	2340	1253	0.09%	0.012%
8	2.859	546	550	554	rBV6	1390	1145	0.09%	0.011%
9	2.881	555	557	559	rVB3	1278	556	0.04%	0.005%
10	2.933	571	573	574	rBV2	1178	531	0.04%	0.005%
11	3.077	612	618	621	rBV7	1911	1717	0.13%	0.016%
12	3.093	621	623	628	rVV5	875	805	0.06%	0.007%
13	3.187	643	652	655	rBV9	1763	2047	0.15%	0.019%
14	3.209	655	659	660	rBV4	688	548	0.04%	0.005%
15	3.280	677	681	683	rBV5	1624	1055	0.08%	0.010%
16	3.360	704	706	708	rBV3	1327	776	0.06%	0.007%
17	3.469	738	740	743	rBV3	916	541	0.04%	0.005%
18	3.518	754	755	758	rBV2	1069	612	0.05%	0.006%
19	3.695	808	810	813	rVV4	1045	588	0.04%	0.005%
20	3.717	813	817	820	rVV4	1355	1248	0.09%	0.012%
21	3.936	865	885	905	rBV3	178588	619999	46.14%	5.771%
22	4.228	973	976	977	rBV3	1608	889	0.07%	0.008%
23	4.376	1008	1022	1043	rBV	234432	540930	40.25%	5.035%
24	4.839	1164	1166	1170	rVV3	1154	615	0.05%	0.006%
25	4.932	1192	1195	1196	rBV3	1216	609	0.05%	0.006%
26	4.942	1196	1198	1201	rVB4	1431	571	0.04%	0.005%
27	5.071	1222	1238	1265	rBV2	518166	1343823	100.00%	12.508%
28	5.370	1329	1331	1334	rBV2	1242	946	0.07%	0.009%
29	5.640	1403	1415	1438	rBV	418736	832633	61.96%	7.750%
30	5.929	1495	1505	1519	rBV3	25882	52942	3.94%	0.493%
31	6.010	1528	1530	1531	rBV2	1362	660	0.05%	0.006%
32	6.093	1539	1556	1575	rBV	303297	623915	46.43%	5.807%
33	6.363	1635	1640	1641	rBV5	1233	1059	0.08%	0.010%
34	6.453	1665	1668	1669	rBV3	1268	612	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016982.D
 Acq On : 18 Jun 2020 17:05
 Operator : SY/MD
 Sample : L3039-01DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M00DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.508	1682	1685	1688	rBV4	1609	1177	0.09%	0.011%
36	6.585	1705	1709	1713	rBV7	1026	778	0.06%	0.007%
37	6.659	1730	1732	1734	rBV3	1820	1090	0.08%	0.010%
38	6.698	1742	1744	1749	rBV5	1247	852	0.06%	0.008%
39	7.006	1829	1840	1860	rBV	177456	320623	23.86%	2.984%
40	7.177	1888	1893	1894	rBV4	1552	1101	0.08%	0.010%
41	7.338	1931	1943	1964	rBV	631903	1085273	80.76%	10.101%
42	7.643	2025	2038	2057	rBV	127968	227118	16.90%	2.114%
43	7.791	2083	2084	2087	rBV3	1260	590	0.04%	0.005%
44	7.997	2144	2148	2149	rBV4	2892	2128	0.16%	0.020%
45	8.035	2158	2160	2165	rVB3	1066	730	0.05%	0.007%
46	8.109	2173	2183	2212	rBV2	304533	609680	45.37%	5.675%
47	8.563	2322	2324	2327	rBV3	1535	1168	0.09%	0.011%
48	8.598	2333	2335	2337	rBV3	1135	492	0.04%	0.005%
49	8.784	2389	2393	2394	rBV3	1695	1115	0.08%	0.010%
50	8.874	2409	2421	2439	rBV	623948	1007210	74.95%	9.375%
51	9.145	2502	2505	2506	rBV3	1752	1083	0.08%	0.010%
52	9.257	2538	2540	2543	rBV4	1284	804	0.06%	0.007%
53	9.286	2545	2549	2552	rVB4	1683	1307	0.10%	0.012%
54	9.305	2552	2555	2557	rVB3	1602	1005	0.07%	0.009%
55	9.347	2565	2568	2570	rBV3	1690	957	0.07%	0.009%
56	9.472	2604	2607	2609	rBV4	1387	843	0.06%	0.008%
57	9.537	2625	2627	2629	rVB3	1376	519	0.04%	0.005%
58	9.566	2630	2636	2639	rBV7	2596	2959	0.22%	0.028%
59	9.726	2682	2686	2688	rBV4	1431	1048	0.08%	0.010%
60	9.804	2705	2710	2713	rBV7	1822	1451	0.11%	0.014%
61	9.868	2728	2730	2732	rVB2	1544	547	0.04%	0.005%
62	9.884	2732	2735	2738	rBV5	1173	697	0.05%	0.006%
63	9.939	2748	2752	2755	rBV5	1177	1188	0.09%	0.011%
64	10.132	2808	2812	2817	rBV6	905	1048	0.08%	0.010%
65	10.238	2832	2845	2857	rBV	385841	601777	44.78%	5.601%
66	10.421	2899	2902	2904	rBV4	1778	1299	0.10%	0.012%
67	10.479	2916	2920	2923	rBV3	1349	1130	0.08%	0.011%
68	10.546	2938	2941	2947	rBV7	1612	1954	0.15%	0.018%
69	10.649	2969	2973	2975	rBV5	1300	829	0.06%	0.008%
70	10.698	2985	2988	2991	rBV4	861	636	0.05%	0.006%
71	10.932	3058	3061	3063	rBV4	2416	1809	0.13%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016982.D
 Acq On : 18 Jun 2020 17:05
 Operator : SY/MD
 Sample : L3039-01DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M00DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.971	3071	3073	3077	rVB5	1819	1175	0.09%	0.011%
73	10.990	3077	3079	3085	rVB7	1915	1469	0.11%	0.014%
74	11.025	3085	3090	3093	rBV6	1529	1673	0.12%	0.016%
75	11.141	3122	3126	3130	rBV6	1459	1559	0.12%	0.015%
76	11.164	3130	3133	3137	rVB5	1536	1361	0.10%	0.013%
77	11.270	3155	3166	3184	rBV	634352	960806	71.50%	8.943%
78	11.527	3244	3246	3250	rVB5	1008	731	0.05%	0.007%
79	11.553	3250	3254	3256	rBV4	2209	1871	0.14%	0.017%
80	11.646	3267	3283	3302	rBV	670642	1046447	77.87%	9.740%
81	11.781	3323	3325	3328	rBV4	1382	885	0.07%	0.008%
82	12.119	3427	3430	3439	rBV10	1479	1830	0.14%	0.017%
83	12.379	3509	3511	3513	rBV2	1159	589	0.04%	0.005%
84	12.456	3531	3535	3537	rBV3	1422	984	0.07%	0.009%
85	12.469	3537	3539	3540	rBV2	1720	665	0.05%	0.006%
86	12.662	3594	3599	3601	rBV4	2650	2231	0.17%	0.021%
87	12.787	3636	3638	3641	rBV3	1131	766	0.06%	0.007%
88	12.855	3654	3659	3661	rBV5	2573	2584	0.19%	0.024%
89	12.897	3670	3672	3675	rVB3	1327	607	0.05%	0.006%
90	12.945	3683	3687	3691	rVB6	1761	1657	0.12%	0.015%
91	12.971	3693	3695	3703	rVB7	1155	1323	0.10%	0.012%
92	13.083	3728	3730	3733	rBV4	1199	692	0.05%	0.006%
93	13.691	3917	3919	3921	rBV3	1304	647	0.05%	0.006%
94	13.765	3937	3942	3943	rBV3	3713	2627	0.20%	0.024%
95	13.810	3954	3956	3959	rBV4	1235	711	0.05%	0.007%
96	14.160	4060	4065	4066	rBV4	1927	1353	0.10%	0.013%
97	14.662	4217	4221	4223	rVB4	1860	981	0.07%	0.009%
98	14.675	4223	4225	4227	rBV4	1694	665	0.05%	0.006%
99	15.006	4325	4328	4333	rBV6	2131	2153	0.16%	0.020%
100	15.758	4560	4562	4565	rBV3	1779	1223	0.09%	0.011%


Sum of corrected areas: 10744119

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016982.D
Acq On : 18 Jun 2020 17:05
Operator : SY/MD
Sample : L3039-01DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M00DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

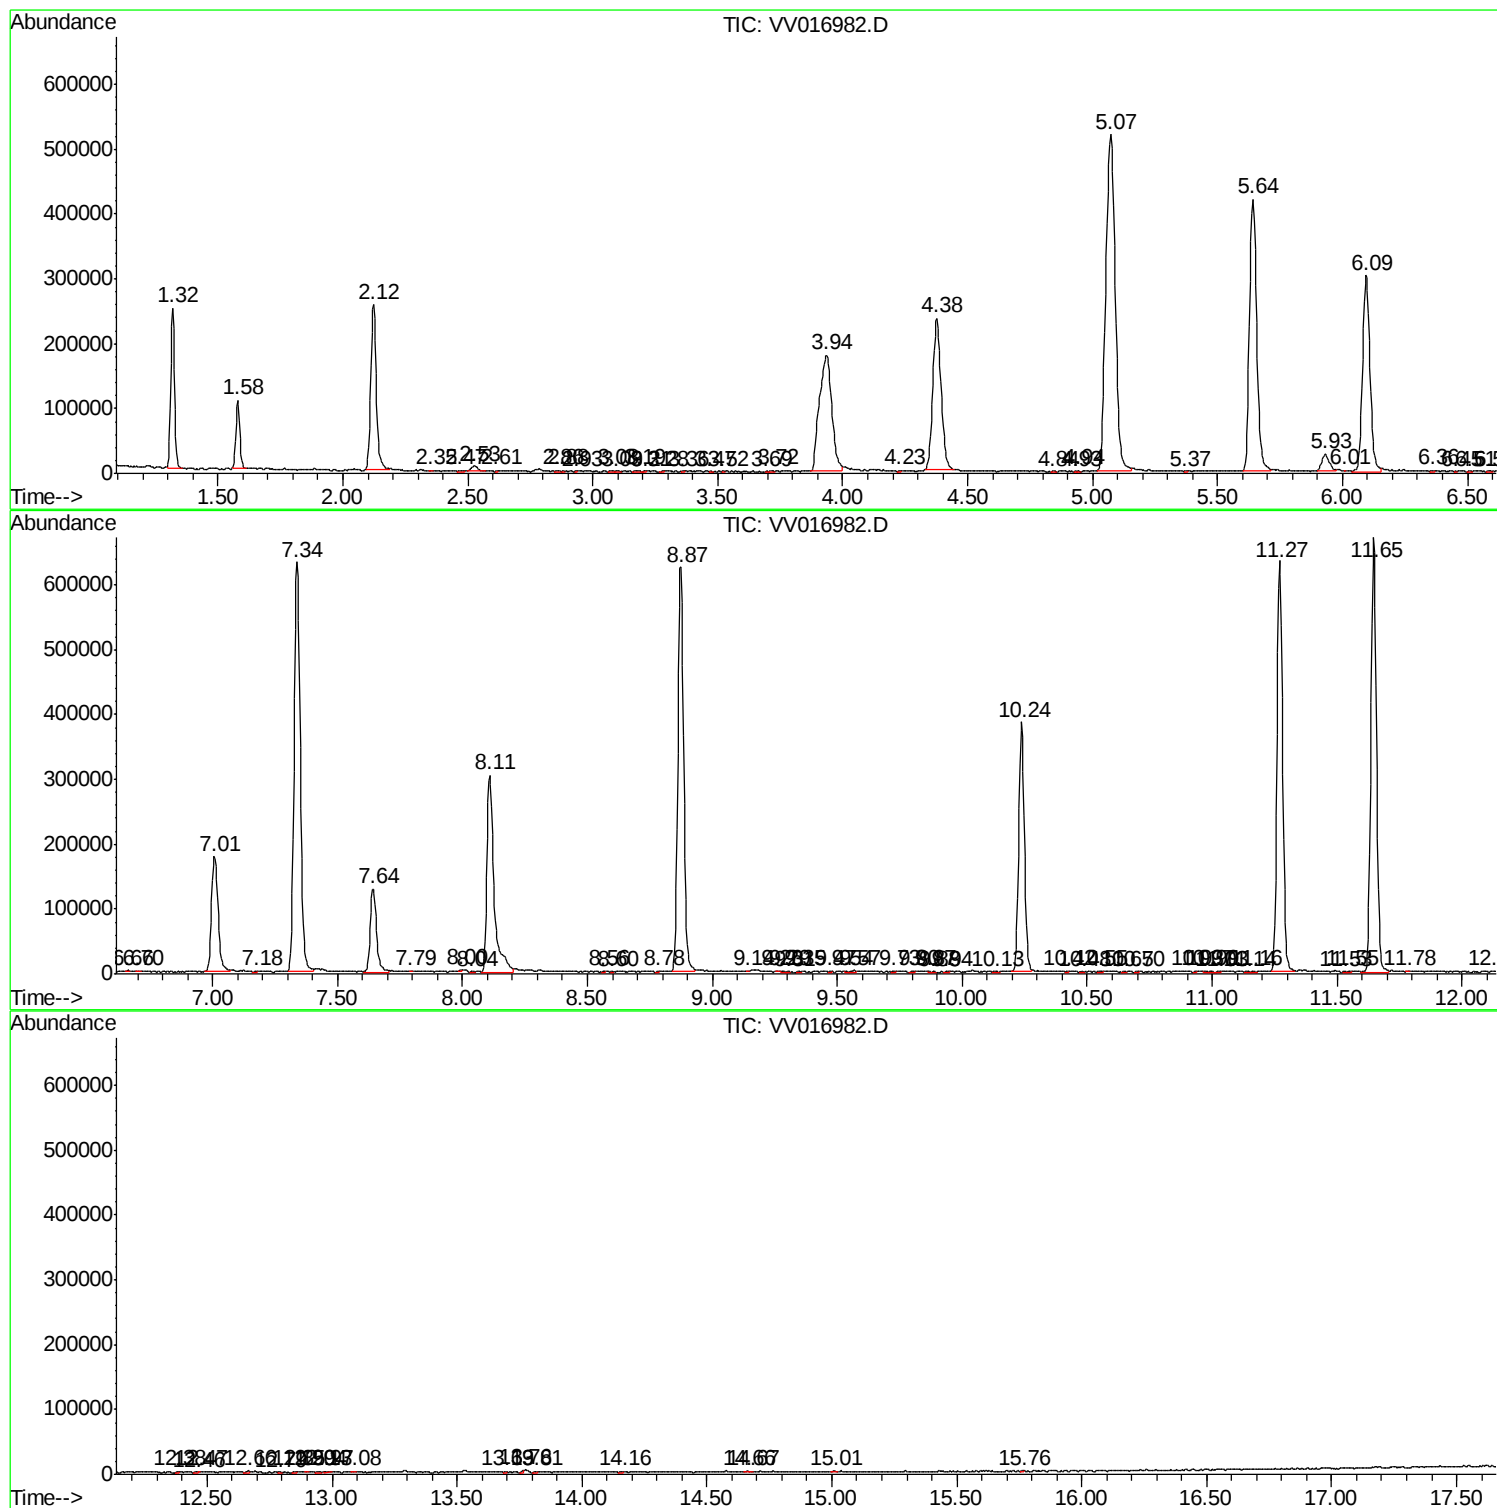

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016982.D
Acq On : 18 Jun 2020 17:05
Operator : SY/MD
Sample : L3039-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M00DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016982.D
Acq On : 18 Jun 2020 17:05
Operator : SY/MD
Sample : L3039-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M00DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc