

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016984.D
 Acq On : 18 Jun 2020 17:52
 Operator : SY/MD
 Sample : L3039-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	144928	149612	11.10%	1.404%
2	1.579	146	152	163	rVB	103350	117702	8.73%	1.104%
3	2.123	312	321	340	rVB	248960	376505	27.94%	3.532%
4	2.576	458	462	465	rBV6	1151	985	0.07%	0.009%
5	2.602	468	470	473	rBV4	1404	910	0.07%	0.009%
6	2.618	473	475	477	rBV3	1030	577	0.04%	0.005%
7	2.676	491	493	495	rBV3	1299	591	0.04%	0.006%
8	2.840	542	544	548	rBV5	1308	744	0.06%	0.007%
9	2.926	569	571	574	rBV4	1073	489	0.04%	0.005%
10	3.058	610	612	613	rBV2	1393	626	0.05%	0.006%
11	3.126	632	633	635	rBV2	817	351	0.03%	0.003%
12	3.184	648	651	655	rVB5	1359	900	0.07%	0.008%
13	3.222	662	663	666	rVB3	1305	384	0.03%	0.004%
14	3.248	666	671	677	rBV9	1875	2350	0.17%	0.022%
15	3.328	692	696	698	rBV4	1143	677	0.05%	0.006%
16	3.341	698	700	704	rVV4	1122	852	0.06%	0.008%
17	3.370	707	709	712	rVB3	1518	878	0.07%	0.008%
18	3.386	712	714	716	rBV2	1456	870	0.06%	0.008%
19	3.450	731	734	735	rBV3	790	480	0.04%	0.005%
20	3.544	761	763	764	rBV2	1411	685	0.05%	0.006%
21	3.682	802	806	810	rBV6	1423	1325	0.10%	0.012%
22	3.724	815	819	820	rBV3	1105	673	0.05%	0.006%
23	3.749	825	827	828	rBV2	659	267	0.02%	0.003%
24	3.769	831	833	835	rVV3	680	228	0.02%	0.002%
25	3.801	841	843	849	rVB5	1248	941	0.07%	0.009%
26	3.836	851	854	856	rBV3	1641	853	0.06%	0.008%
27	3.936	866	885	911	rBV2	256371	816340	60.58%	7.659%
28	4.376	1008	1022	1045	rVB	221767	536870	39.84%	5.037%
29	4.627	1098	1100	1102	rBV3	1412	540	0.04%	0.005%
30	5.071	1221	1238	1265	rBV2	525658	1347482	100.00%	12.642%
31	5.402	1339	1341	1346	rVB5	1995	1176	0.09%	0.011%
32	5.540	1382	1384	1387	rVB3	1431	822	0.06%	0.008%
33	5.566	1387	1392	1394	rBV6	1777	1669	0.12%	0.016%
34	5.595	1398	1401	1402	rBV3	1407	683	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016984.D
 Acq On : 18 Jun 2020 17:52
 Operator : SY/MD
 Sample : L3039-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1402	1415	1439	rBV	422263	839289	62.29%	7.874%
36	6.093	1544	1556	1579	rVB	303035	604223	44.84%	5.669%
37	6.344	1632	1634	1640	rBV6	1756	1474	0.11%	0.014%
38	6.479	1674	1676	1678	rBV3	946	414	0.03%	0.004%
39	6.534	1690	1693	1697	rBV4	1643	1231	0.09%	0.012%
40	6.611	1711	1717	1721	rBV7	2045	1994	0.15%	0.019%
41	6.817	1779	1781	1783	rBV2	779	339	0.03%	0.003%
42	6.862	1793	1795	1796	rBV2	1107	552	0.04%	0.005%
43	6.907	1805	1809	1812	rBV6	1017	1047	0.08%	0.010%
44	6.942	1818	1820	1822	rBV3	885	423	0.03%	0.004%
45	7.007	1830	1840	1862	rBV2	174087	311078	23.09%	2.919%
46	7.338	1931	1943	1962	rBV	625501	1066467	79.15%	10.006%
47	7.643	2028	2038	2058	rBV	124669	211885	15.72%	1.988%
48	8.042	2160	2162	2166	rBV3	1441	1002	0.07%	0.009%
49	8.071	2169	2171	2172	rBV2	1212	471	0.03%	0.004%
50	8.109	2173	2183	2214	rVV2	296651	589466	43.75%	5.530%
51	8.566	2323	2325	2328	rBV3	1226	773	0.06%	0.007%
52	8.733	2376	2377	2379	rBV2	1082	581	0.04%	0.005%
53	8.871	2408	2420	2438	rBV	626094	1016791	75.46%	9.539%
54	9.486	2609	2611	2613	rBV2	763	258	0.02%	0.002%
55	9.836	2718	2720	2727	rBV8	1171	916	0.07%	0.009%
56	9.961	2757	2759	2762	rBV4	1332	661	0.05%	0.006%
57	10.003	2770	2772	2779	rBV8	1242	841	0.06%	0.008%
58	10.055	2787	2788	2789	rBV	1291	396	0.03%	0.004%
59	10.097	2795	2801	2804	rBV7	1836	2125	0.16%	0.020%
60	10.161	2817	2821	2826	rBV6	1383	1499	0.11%	0.014%
61	10.190	2826	2830	2831	rBV3	961	597	0.04%	0.006%
62	10.238	2834	2845	2858	rVV	382916	594764	44.14%	5.580%
63	10.463	2912	2915	2916	rBV2	1112	615	0.05%	0.006%
64	10.588	2951	2954	2955	rBV2	1584	834	0.06%	0.008%
65	10.656	2971	2975	2977	rBV4	941	852	0.06%	0.008%
66	10.723	2994	2996	2997	rBV2	1242	632	0.05%	0.006%
67	10.897	3047	3050	3055	rVB7	1433	1416	0.11%	0.013%
68	10.926	3055	3059	3060	rBV4	1585	1240	0.09%	0.012%
69	10.939	3060	3063	3068	rVB6	2412	2335	0.17%	0.022%
70	11.122	3118	3120	3121	rBV2	847	344	0.03%	0.003%
71	11.170	3133	3135	3138	rBV4	1266	812	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016984.D
 Acq On : 18 Jun 2020 17:52
 Operator : SY/MD
 Sample : L3039-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3186	rBV	625807	969980	71.98%	9.100%
73	11.646	3271	3283	3301	rBV	663029	1034128	76.75%	9.702%
74	11.891	3357	3359	3363	rBV5	2429	1766	0.13%	0.017%
75	12.029	3398	3402	3406	rBV6	1760	1967	0.15%	0.018%
76	12.080	3416	3418	3422	rBV3	1087	751	0.06%	0.007%
77	12.225	3459	3463	3466	rVB5	1132	689	0.05%	0.006%
78	12.576	3569	3572	3574	rBV4	1768	971	0.07%	0.009%
79	12.637	3589	3591	3593	rVB2	1051	458	0.03%	0.004%
80	12.727	3615	3619	3620	rBV3	1180	818	0.06%	0.008%
81	12.833	3649	3652	3656	rBV5	1636	1203	0.09%	0.011%
82	12.945	3684	3687	3692	rBV6	1816	1646	0.12%	0.015%
83	12.977	3695	3697	3702	rVB5	1189	878	0.07%	0.008%
84	13.064	3721	3724	3727	rBV4	1473	1029	0.08%	0.010%
85	13.090	3730	3732	3733	rBV2	1515	593	0.04%	0.006%
86	13.219	3770	3772	3774	rBV3	1617	819	0.06%	0.008%
87	13.665	3909	3911	3914	rBV2	1593	996	0.07%	0.009%
88	13.784	3946	3948	3954	rVB6	1984	1353	0.10%	0.013%
89	13.839	3963	3965	3968	rBV4	1220	861	0.06%	0.008%
90	13.900	3982	3984	3987	rBV4	1196	716	0.05%	0.007%
91	14.026	4021	4023	4026	rBV3	1216	583	0.04%	0.005%
92	14.042	4026	4028	4031	rVV3	1176	751	0.06%	0.007%
93	14.058	4031	4033	4039	rVB6	2183	1673	0.12%	0.016%
94	14.280	4100	4102	4105	rBV4	1425	771	0.06%	0.007%
95	14.402	4137	4140	4142	rBV3	1163	661	0.05%	0.006%
96	14.514	4172	4175	4178	rBV3	1337	925	0.07%	0.009%
97	14.778	4255	4257	4260	rBV3	945	478	0.04%	0.004%
98	14.891	4289	4292	4296	rBV4	1981	1645	0.12%	0.015%
99	15.058	4342	4344	4347	rBV4	1635	1261	0.09%	0.012%
100	15.312	4421	4423	4424	rBV2	1731	712	0.05%	0.007%


Sum of corrected areas: 10658756

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016984.D
Acq On : 18 Jun 2020 17:52
Operator : SY/MD
Sample : L3039-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

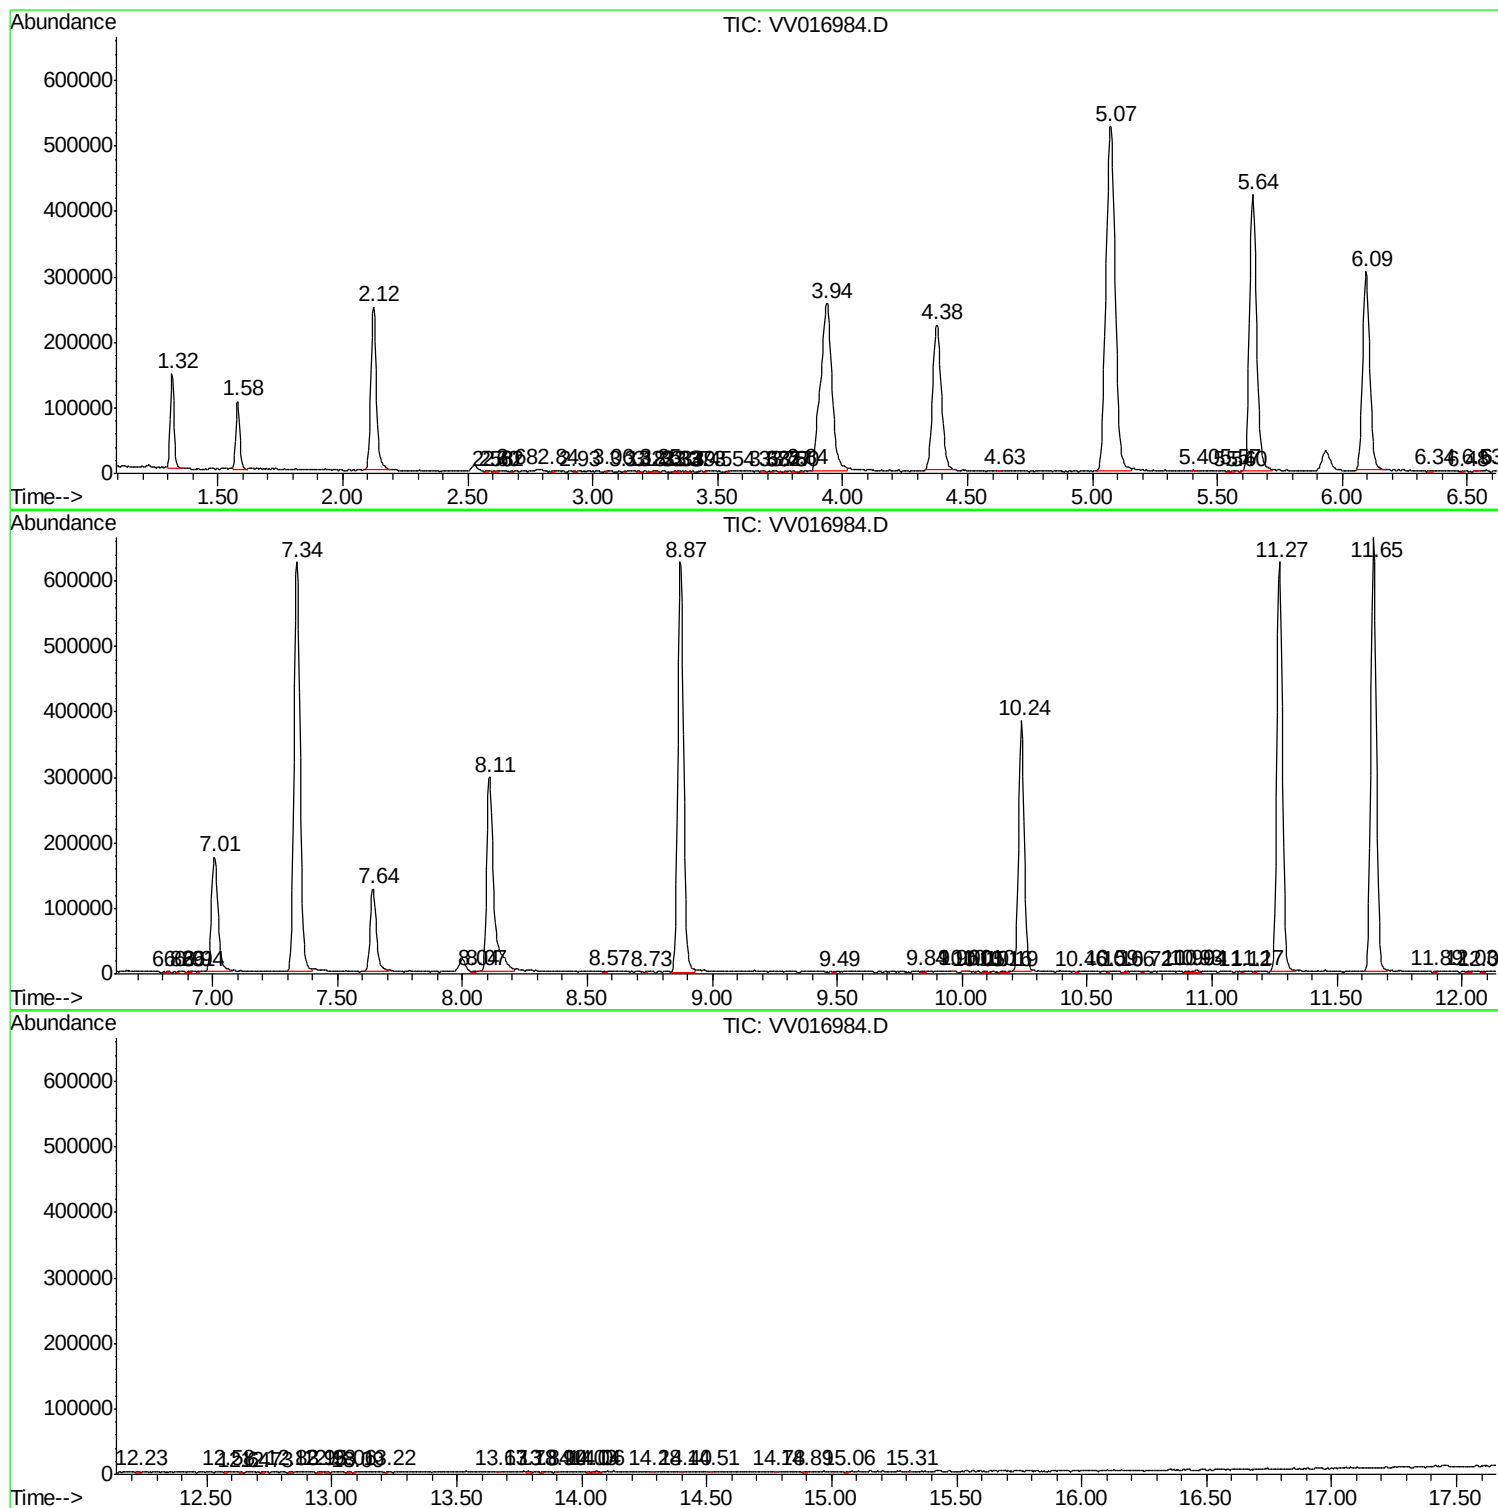

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016984.D
Acq On : 18 Jun 2020 17:52
Operator : SY/MD
Sample : L3039-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061820\
Data File : VV016984.D
Acq On : 18 Jun 2020 17:52
Operator : SY/MD
Sample : L3039-03DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9M02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc