

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016987.D
 Acq On : 18 Jun 2020 19:01
 Operator : SY/MD
 Sample : L3039-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	140057	138433	7.82%	1.157%
2	1.579	145	152	163	rVB	107962	118501	6.69%	0.991%
3	2.123	312	321	338	rBV	244342	357663	20.20%	2.991%
4	2.293	370	374	378	rBV6	2050	2032	0.11%	0.017%
5	2.878	552	556	560	rBV7	1686	1514	0.09%	0.013%
6	2.904	560	564	566	rBV4	1243	769	0.04%	0.006%
7	2.978	585	587	592	rVV5	1286	1102	0.06%	0.009%
8	3.135	634	636	640	rVV4	1070	903	0.05%	0.008%
9	3.190	651	653	656	rBV3	1407	935	0.05%	0.008%
10	3.479	741	743	747	rVB4	1320	870	0.05%	0.007%
11	3.508	747	752	753	rBV4	945	767	0.04%	0.006%
12	3.666	798	801	805	rVB5	1330	1064	0.06%	0.009%
13	3.737	819	823	826	rBV3	1259	1067	0.06%	0.009%
14	3.788	836	839	842	rBV5	1684	1023	0.06%	0.009%
15	3.926	867	882	908	rBV4	112414	428428	24.19%	3.582%
16	4.254	982	984	987	rVB3	1607	760	0.04%	0.006%
17	4.286	990	994	999	rBV7	1820	1712	0.10%	0.014%
18	4.376	1008	1022	1043	rBV	219060	518003	29.25%	4.331%
19	4.682	1115	1117	1122	rVB6	1938	1399	0.08%	0.012%
20	4.827	1160	1162	1164	rBV3	1909	944	0.05%	0.008%
21	4.917	1188	1190	1192	rBV2	1624	939	0.05%	0.008%
22	4.929	1192	1194	1198	rVB5	1459	998	0.06%	0.008%
23	5.074	1221	1239	1262	rBV2	505395	1307886	73.86%	10.936%
24	5.476	1360	1364	1366	rBV4	1633	1281	0.07%	0.011%
25	5.537	1381	1383	1389	rBV8	1747	1339	0.08%	0.011%
26	5.640	1401	1415	1435	rBV	406797	812208	45.87%	6.791%
27	5.939	1492	1508	1526	rBV2	77769	175367	9.90%	1.466%
28	6.093	1544	1556	1578	rVB	292662	593982	33.54%	4.966%
29	6.322	1624	1627	1630	rBV4	1785	1348	0.08%	0.011%
30	6.431	1658	1661	1662	rBV2	1414	908	0.05%	0.008%
31	6.759	1758	1763	1764	rBV3	1233	800	0.05%	0.007%
32	6.810	1777	1779	1783	rBV4	1809	1146	0.06%	0.010%
33	6.846	1785	1790	1792	rBV3	1593	1347	0.08%	0.011%
34	6.878	1796	1800	1804	rBV5	2333	2425	0.14%	0.020%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016987.D
 Acq On : 18 Jun 2020 19:01
 Operator : SY/MD
 Sample : L3039-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.939	1815	1819	1824	rVB8	1623	1516	0.09%	0.013%
36	7.007	1828	1840	1858	rBV	167654	304751	17.21%	2.548%
37	7.338	1931	1943	1962	rBV	603575	1039292	58.69%	8.690%
38	7.643	2026	2038	2056	rBV	120057	210335	11.88%	1.759%
39	7.997	2137	2148	2164	rVB	1070253	1770802	100.00%	14.806%
40	8.109	2172	2183	2214	rBV	300034	583761	32.97%	4.881%
41	8.370	2261	2264	2267	rVB4	1858	1185	0.07%	0.010%
42	8.447	2286	2288	2291	rBV3	1557	1126	0.06%	0.009%
43	8.797	2392	2397	2399	rBV5	1801	1792	0.10%	0.015%
44	8.871	2407	2420	2439	rBV	601750	982087	55.46%	8.212%
45	9.016	2463	2465	2467	rBV2	1244	762	0.04%	0.006%
46	9.032	2468	2470	2474	rVB4	1927	1126	0.06%	0.009%
47	9.309	2550	2556	2561	rBV9	1563	2021	0.11%	0.017%
48	9.392	2578	2582	2585	rBV3	1219	725	0.04%	0.006%
49	9.415	2585	2589	2591	rBV5	1572	1268	0.07%	0.011%
50	9.428	2591	2593	2596	rVB4	1438	775	0.04%	0.006%
51	9.466	2603	2605	2607	rBV4	1695	900	0.05%	0.008%
52	9.572	2634	2638	2644	rVB8	2304	2121	0.12%	0.018%
53	9.624	2652	2654	2660	rVB7	1948	1474	0.08%	0.012%
54	9.650	2660	2662	2667	rBV4	1567	1561	0.09%	0.013%
55	9.791	2701	2706	2709	rBV5	1485	1333	0.08%	0.011%
56	9.920	2743	2746	2748	rBV3	1450	886	0.05%	0.007%
57	10.042	2780	2784	2786	rBV5	1197	932	0.05%	0.008%
58	10.077	2790	2795	2798	rBV5	946	949	0.05%	0.008%
59	10.093	2798	2800	2805	rVB5	1245	835	0.05%	0.007%
60	10.238	2833	2845	2858	rVV	378072	585500	33.06%	4.896%
61	10.399	2890	2895	2905	rVB7	5869	10062	0.57%	0.084%
62	10.518	2928	2932	2937	rVB8	1632	1720	0.10%	0.014%
63	10.765	3008	3009	3014	rVB4	1465	765	0.04%	0.006%
64	10.788	3014	3016	3021	rBV5	1465	1061	0.06%	0.009%
65	10.820	3024	3026	3030	rBV3	1851	1208	0.07%	0.010%
66	11.064	3094	3102	3104	rBV8	1986	2204	0.12%	0.018%
67	11.206	3144	3146	3151	rBV4	1651	1563	0.09%	0.013%
68	11.270	3154	3166	3182	rBV	605762	925926	52.29%	7.742%
69	11.646	3271	3283	3297	rBV	647812	1003260	56.66%	8.389%
70	11.987	3387	3389	3392	rBV4	1258	904	0.05%	0.008%
71	12.022	3398	3400	3402	rBV2	1383	732	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061820\
 Data File : VV016987.D
 Acq On : 18 Jun 2020 19:01
 Operator : SY/MD
 Sample : L3039-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.119	3428	3430	3433	rBV3	1139	718	0.04%	0.006%
73	12.222	3456	3462	3464	rBV6	1924	1649	0.09%	0.014%
74	12.437	3526	3529	3533	rBV4	1151	1010	0.06%	0.008%
75	12.666	3596	3600	3602	rBV3	1278	1149	0.06%	0.010%
76	12.730	3618	3620	3627	rVB7	1849	1302	0.07%	0.011%
77	12.762	3627	3630	3631	rBV3	1647	940	0.05%	0.008%
78	12.842	3652	3655	3660	rVB6	2092	1617	0.09%	0.014%
79	12.868	3660	3663	3664	rBV3	1431	849	0.05%	0.007%
80	12.945	3685	3687	3691	rBV5	1359	733	0.04%	0.006%
81	12.987	3697	3700	3702	rBV4	1595	926	0.05%	0.008%
82	13.042	3714	3717	3719	rVB5	1356	726	0.04%	0.006%
83	13.061	3719	3723	3725	rBV3	1516	1232	0.07%	0.010%
84	13.174	3755	3758	3761	rBV3	2015	1097	0.06%	0.009%
85	13.264	3784	3786	3789	rVV4	1331	783	0.04%	0.007%
86	13.460	3843	3847	3850	rBV5	1488	1401	0.08%	0.012%
87	13.585	3883	3886	3889	rVB4	1411	785	0.04%	0.007%
88	13.662	3907	3910	3911	rBV2	1475	869	0.05%	0.007%
89	13.759	3936	3940	3942	rBV3	1474	1282	0.07%	0.011%
90	13.865	3969	3973	3977	rBV7	1361	1234	0.07%	0.010%
91	13.884	3977	3979	3981	rBV3	1785	832	0.05%	0.007%
92	14.051	4028	4031	4033	rBV4	1388	784	0.04%	0.007%
93	14.267	4093	4098	4100	rBV4	1550	1093	0.06%	0.009%
94	14.669	4221	4223	4225	rBV3	2243	1245	0.07%	0.010%
95	14.743	4244	4246	4250	rBV4	1293	996	0.06%	0.008%
96	14.829	4271	4273	4277	rBV4	1343	1011	0.06%	0.008%
97	15.161	4372	4376	4378	rBV5	1546	1427	0.08%	0.012%
98	15.276	4407	4412	4414	rBV6	1723	1501	0.08%	0.013%
99	15.665	4531	4533	4535	rBV3	1614	864	0.05%	0.007%
100	15.691	4539	4541	4543	rBV3	1448	732	0.04%	0.006%


Sum of corrected areas: 11959870

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061820\
Data File : VV016987.D
Acq On : 18 Jun 2020 19:01
Operator : SY/MD
Sample : L3039-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9M11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

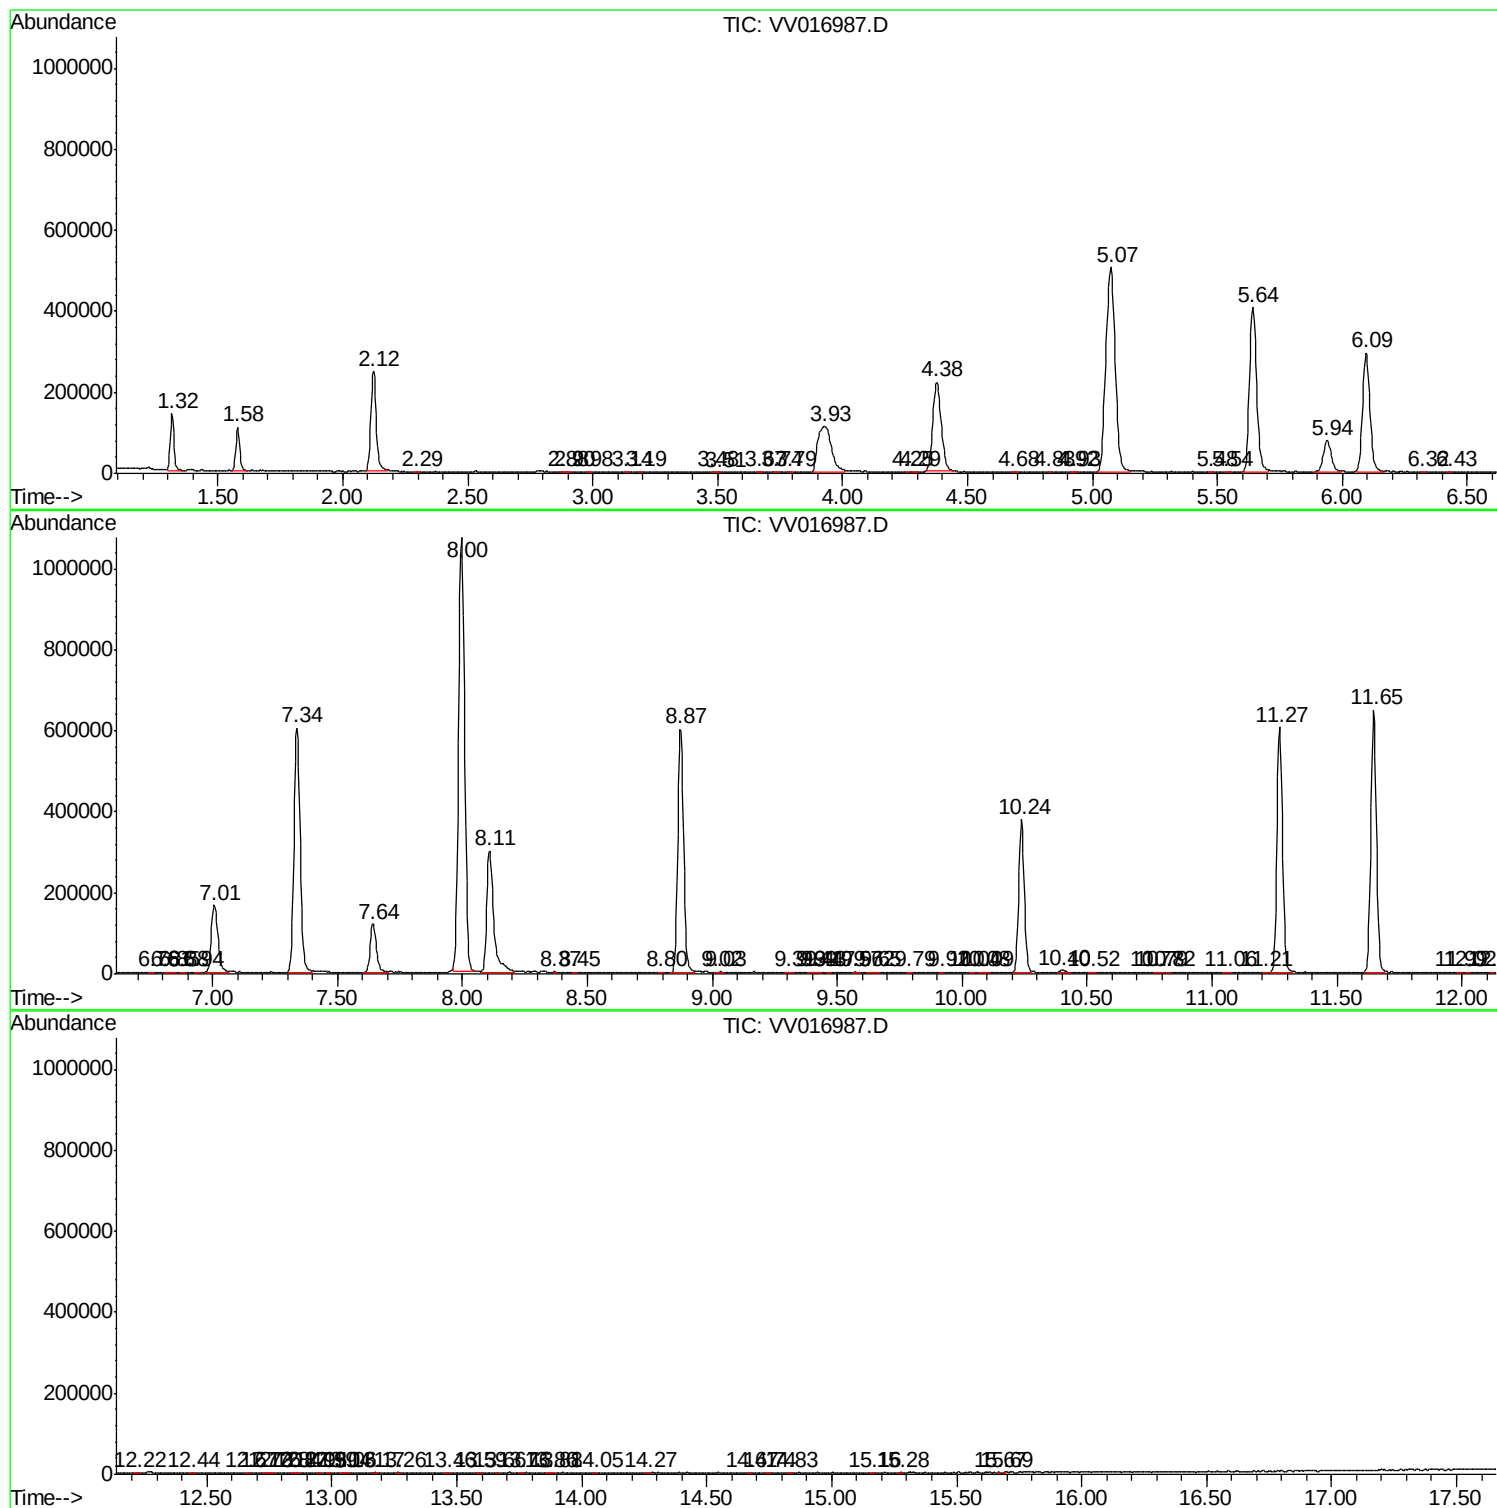

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016987.D
Acq On : 18 Jun 2020 19:01
Operator : SY/MD
Sample : L3039-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061820\
Data File : VV016987.D
Acq On : 18 Jun 2020 19:01
Operator : SY/MD
Sample : L3039-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M11

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
