


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061820\
 Data File : VV016966.D
 Acq On : 18 Jun 2020 08:48
 Operator : SY/MD
 Sample : BFB91
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB91

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 19 06:58:06 2020

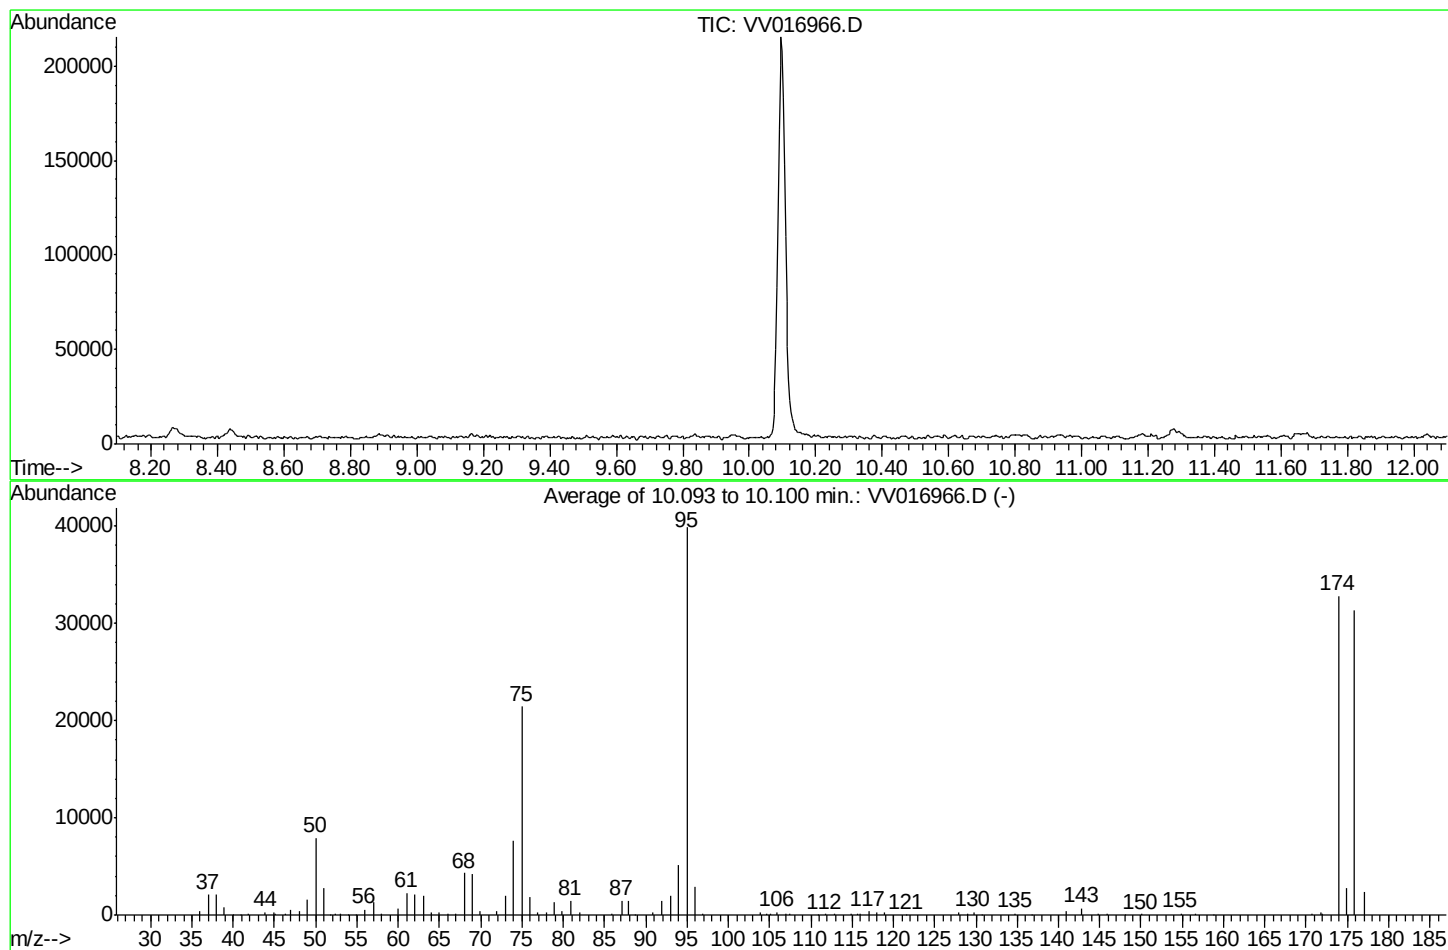

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	7939	PASS
75	95	30	80	53.8	21461	PASS
95	95	100	100	100.0	39882	PASS
96	95	5	9	7.4	2962	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.4	32856	PASS
175	174	5	9	8.4	2770	PASS
176	174	95	101	95.4	31333	PASS
177	176	5	9	7.6	2375	PASS

m/z	Abundance
35.90	492.0
37.00	2061.0
38.00	1954.0
39.00	818.0
39.90	442.0
40.90	148.0
41.70	159.0
43.10	138.0
43.90	692.0
44.90	509.0
45.80	175.0
46.30	157.0
47.00	619.0
47.90	371.0
49.00	1525.0
50.00	7497.0
51.00	2784.0
51.90	139.0
52.30	156.0
53.00	115.0
54.90	153.0
56.00	725.0
57.00	1282.0
59.90	655.0
61.00	2258.0
62.00	2026.0
63.00	1861.0
64.00	286.0
65.00	310.0
65.90	125.0
67.00	179.0
68.00	4143.0
69.00	4277.0
69.90	402.0
71.80	335.0
73.00	1898.0
74.00	7178.0
75.00	20424.0
76.00	1769.0
77.00	276.0
77.90	207.0
78.90	1295.0
79.80	450.0
80.80	1451.0
81.90	329.0
85.90	133.0
87.00	1711.0
87.90	1480.0
90.90	194.0
92.00	1379.0
93.00	2115.0
94.00	5018.0
95.00	38800.0
96.00	3033.0
96.90	179.0
103.90	253.0
104.60	144.0
105.00	140.0
105.90	306.0
107.00	147.0
110.80	120.0
112.90	139.0
114.90	126.0
115.70	177.0
117.00	336.0
117.90	230.0
118.80	266.0
128.00	233.0
129.00	127.0
129.70	345.0
134.80	216.0
136.80	138.0
140.90	434.0
142.80	661.0
144.70	143.0
145.90	106.0
150.00	111.0
154.80	164.0
156.70	156.0
170.90	110.0
171.80	478.0
173.90	30888.0
174.90	2221.0
175.90	29896.0
177.00	2414.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.90	488.0
37.00	2205.0
38.00	2152.0
39.00	938.0
39.90	404.0
40.80	138.0
41.80	157.0
43.00	175.0
43.90	709.0
44.90	527.0
46.20	216.0
47.00	582.0
47.90	349.0
49.00	1721.0
50.00	8164.0
51.00	2871.0
51.90	177.0
52.30	207.0
53.00	112.0
55.00	157.0
55.90	688.0
57.00	1372.0
57.90	114.0
59.90	624.0
61.00	2374.0
62.00	2223.0
63.00	2009.0
64.00	282.0
65.00	348.0
65.90	138.0
67.00	186.0
68.00	4453.0
69.00	4433.0
69.90	423.0
71.80	359.0
73.00	2081.0
74.00	7880.0
75.00	22184.0
76.00	1815.0
77.00	236.0
77.90	226.0
78.90	1399.0
79.80	487.0
80.80	1549.0
81.90	344.0
85.90	117.0
87.00	1486.0
87.90	1722.0
90.80	251.0
92.00	1469.0
92.90	2061.0
94.00	5286.0
95.00	41184.0
96.00	3111.0
96.90	131.0
103.90	251.0
104.60	125.0
105.10	158.0
105.90	288.0
106.90	156.0
107.40	128.0
111.70	105.0
112.90	104.0
114.90	110.0
115.70	194.0
116.00	202.0
117.00	331.0
117.90	240.0
118.80	215.0
121.60	102.0
127.90	223.0
129.00	140.0
129.70	294.0
130.70	104.0
134.80	181.0
140.90	473.0
142.90	687.0
144.80	106.0
145.80	120.0
150.00	132.0
154.90	169.0
156.60	187.0
170.70	106.0
171.80	504.0
173.90	34056.0
175.00	2853.0
175.90	32360.0
177.00	2496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.20	109.0
35.90	372.0
37.00	2002.0
38.00	2160.0
39.00	1011.0
39.90	355.0
40.80	139.0
42.00	161.0
42.90	184.0
43.90	681.0
45.10	469.0
46.20	227.0
47.00	488.0
48.00	296.0
49.00	1675.0
50.00	8157.0
51.00	2698.0
51.90	184.0
52.30	234.0
53.00	122.0
53.90	129.0
54.90	173.0
55.90	620.0
57.00	1311.0
57.90	124.0
60.00	549.0
61.00	2105.0
62.00	2221.0
63.00	1881.0
63.90	297.0
65.00	321.0
66.00	171.0
67.00	185.0
68.00	4266.0
69.00	4098.0
69.90	378.0
71.90	335.0
73.00	1968.0
74.00	7685.0
75.00	21776.0
76.00	1799.0
76.90	188.0
77.90	191.0
78.90	1276.0
79.80	418.0
80.90	1474.0
82.00	322.0
85.80	112.0
87.10	1211.0
88.00	1533.0
88.70	112.0
90.80	273.0
91.90	1455.0
92.90	1684.0
94.00	4982.0
95.00	39664.0
96.00	2743.0
103.90	275.0
104.60	105.0
105.20	138.0
105.90	262.0
106.80	161.0
107.40	119.0
111.80	120.0
115.70	180.0
116.00	195.0
117.00	342.0
118.00	218.0
118.90	177.0
127.90	182.0
128.80	143.0
129.80	197.0
134.70	139.0
140.90	446.0
142.90	670.0
145.80	111.0
148.00	102.0
150.10	128.0
154.90	178.0
156.60	152.0
158.80	122.0
170.60	120.0
172.00	503.0
173.90	33624.0
175.00	3238.0
175.90	31744.0
177.00	2216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.00	187.0
36.30	111.0
37.30	107.0
38.90	155.0
40.00	366.0
41.00	107.0
41.20	107.0
42.20	149.0
43.10	182.0
43.90	424.0
44.80	134.0
46.00	107.0
47.70	113.0
48.50	134.0
49.10	119.0
51.70	126.0
53.30	113.0
54.20	113.0
54.80	139.0
55.90	120.0
68.60	112.0
72.70	109.0
79.90	100.0
88.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91