


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061825\
Data File : VV038810.D
Acq On : 18 Jun 2025 09:41
Operator : SY/MD
Sample : BFB237
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB237

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM061625.M
Title : TRACE VOA SOM01.0
Last Update : Wed Jun 18 12:17:29 2025

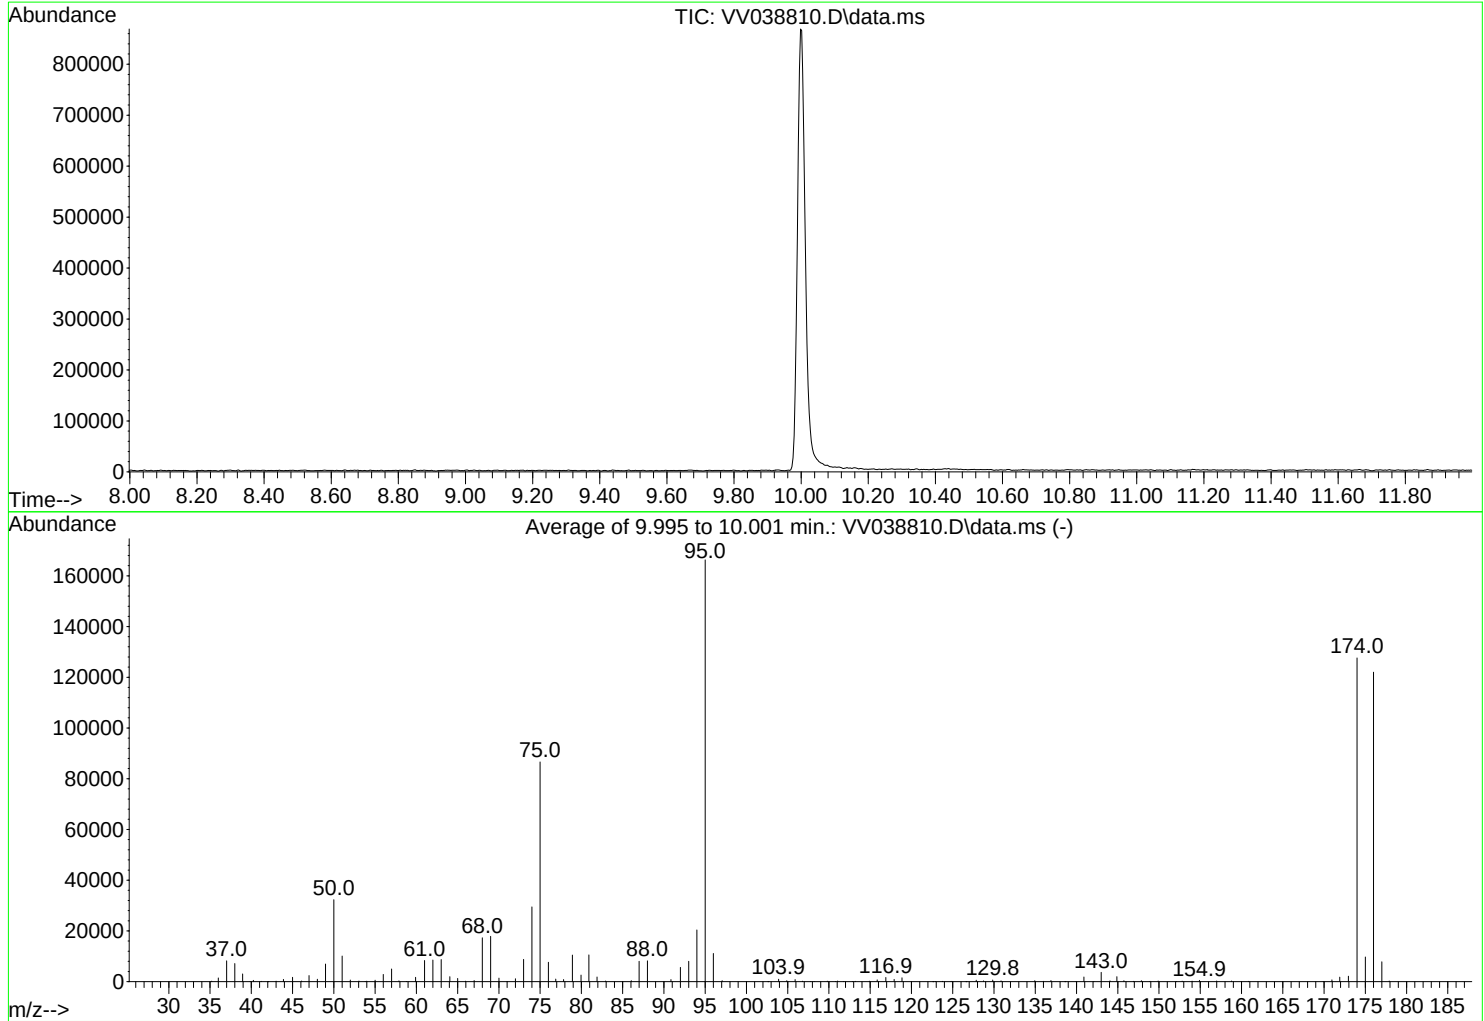

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	32315	PASS
75	95	30	80	52.1	86592	PASS
95	95	100	100	100.0	166293	PASS
96	95	5	9	6.7	11090	PASS
173	174	0.00	2	1.7	2145	PASS
174	95	50	120	76.8	127635	PASS
175	174	5	9	7.6	9693	PASS
176	174	95	101	95.6	121987	PASS
177	176	5	9	6.4	7838	PASS