

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061919\
 Data File : VV011582.D
 Acq On : 18 Jun 2019 18:36
 Operator : SY/MD
 Sample : K3289-14DL 4X
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCL1DL

Quant Time: Jun 19 02:42:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 19 02:08:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	152405	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	142724	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	55327	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	50032	4.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.00%
7) Chloroethane-d5	1.58	69	40361	5.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.60%
11) 1,1-Dichloroethene-d2	2.12	63	82030	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.96	46	191383	59.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.22%
24) Chloroform-d	4.40	84	115831	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
26) 1,2-Dichloroethane-d4	5.08	65	71091	5.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.20%
32) Benzene-d6	5.09	84	225116	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
36) 1,2-Dichloropropane-d6	6.12	67	73370	5.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.60%
41) Toluene-d8	7.36	98	186593	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
43) trans-1,3-Dichloropropene-	7.67	79	22744	5.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.20%
46) 2-Hexanone-d5	8.14	63	143186	55.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	52123	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	61601	5.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.60%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	66282	5.575 ug/L	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061919\
Data File : VV011582.D
Acq On : 18 Jun 2019 18:36
Operator : SY/MD
Sample : K3289-14DL 4X
Misc : 25ML/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCL1DL

Quant Time: Jun 19 02:42:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 19 02:08:53 2019
Response via : Initial Calibration

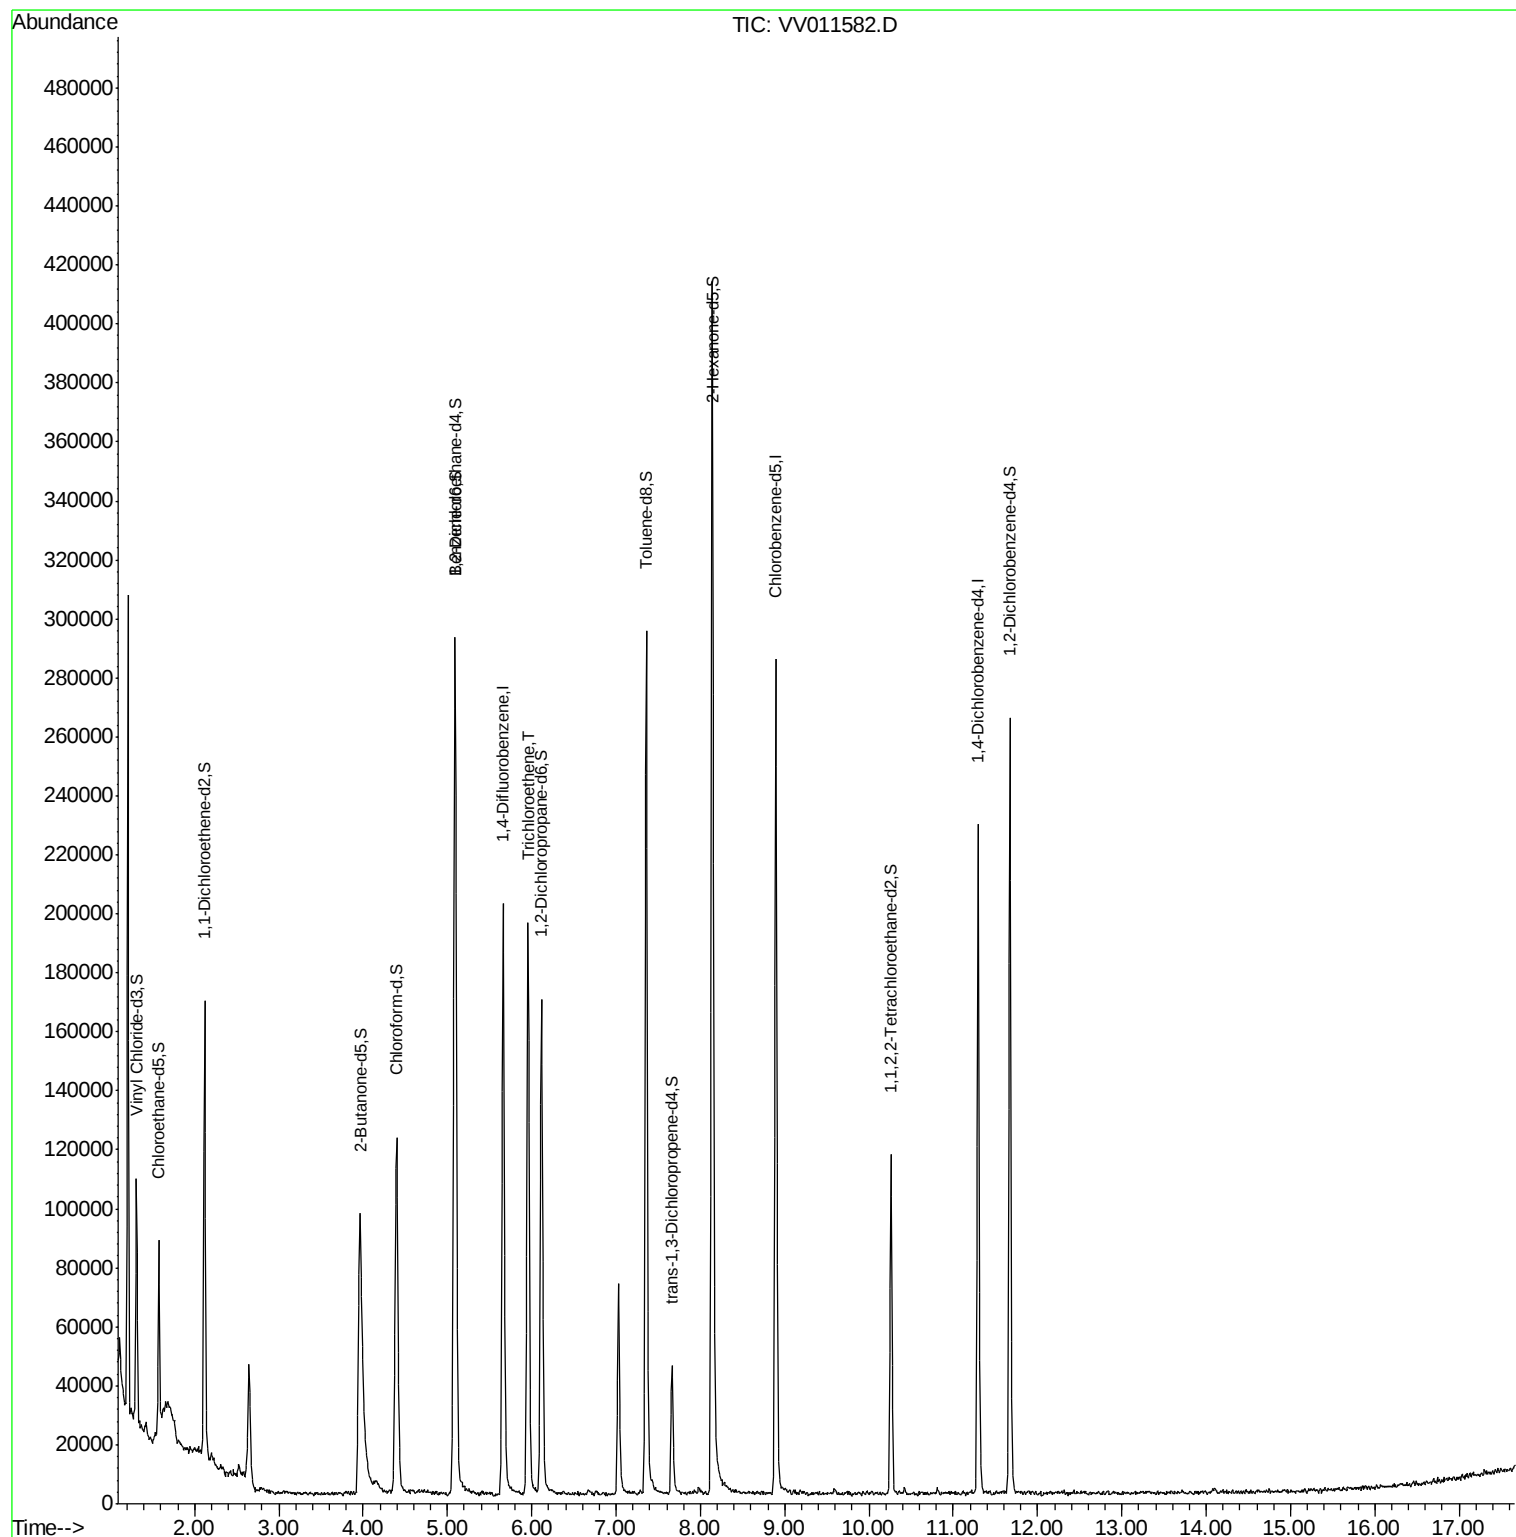

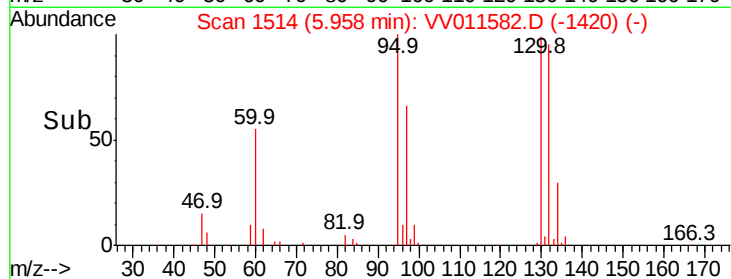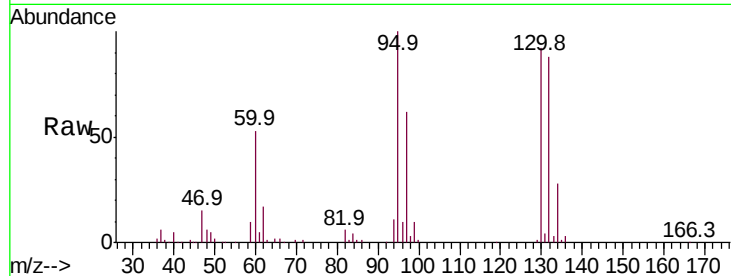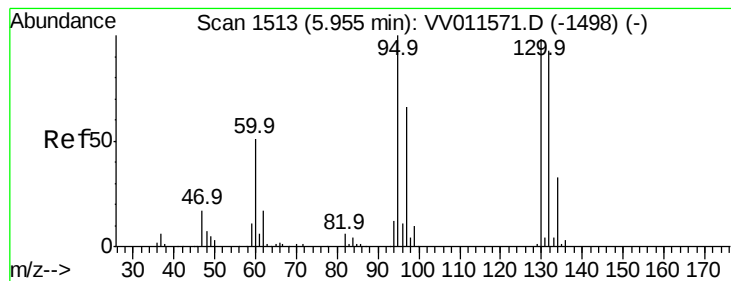

#34

Trichloroethene

Concen: 5.575 ug/L

RT: 5.96 min Scan# 1514

Delta R.T. 0.00 min

Lab File: VV011582.D

Acq: 18 Jun 2019 18:36

Instrument :

MSVOA_V

ClientSampleId :

BFCL1DL

Tot Ion: 95 Resp: 66282

Ion Ratio Lower Upper

95 100

97 61.7 44.4 82.4

132 88.3 63.5 117.9

130 92.1 68.5 127.3

