

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061919\
 Data File : VV011586.D
 Acq On : 18 Jun 2019 20:20
 Operator : SY/MD
 Sample : K3381-15
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFC9

Quant Time: Jun 19 02:52:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 19 02:08:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	155959	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	140792	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	53983	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	52189	4.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.60%
7) Chloroethane-d5	1.58	69	40250	5.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.80%
11) 1,1-Dichloroethene-d2	2.12	63	84420	3.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.20%
20) 2-Butanone-d5	3.96	46	190664	57.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.08%
24) Chloroform-d	4.40	84	114696	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.08	65	70540	5.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.80%
32) Benzene-d6	5.09	84	230544	5.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.80%
36) 1,2-Dichloropropane-d6	6.12	67	73201	5.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.80%
41) Toluene-d8	7.36	98	191193	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
43) trans-1,3-Dichloropropene-	7.66	79	21739	4.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.00%
46) 2-Hexanone-d5	8.14	63	143300	55.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.94%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51846	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	63192	5.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.40%


Target Compounds					Ovalue
13) Acetone	2.22	43	6894	3.087 ug/L	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061919\
Data File : VV011586.D
Acq On : 18 Jun 2019 20:20
Operator : SY/MD
Sample : K3381-15
Misc : 25ML/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCS9

Quant Time: Jun 19 02:52:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 19 02:08:53 2019
Response via : Initial Calibration

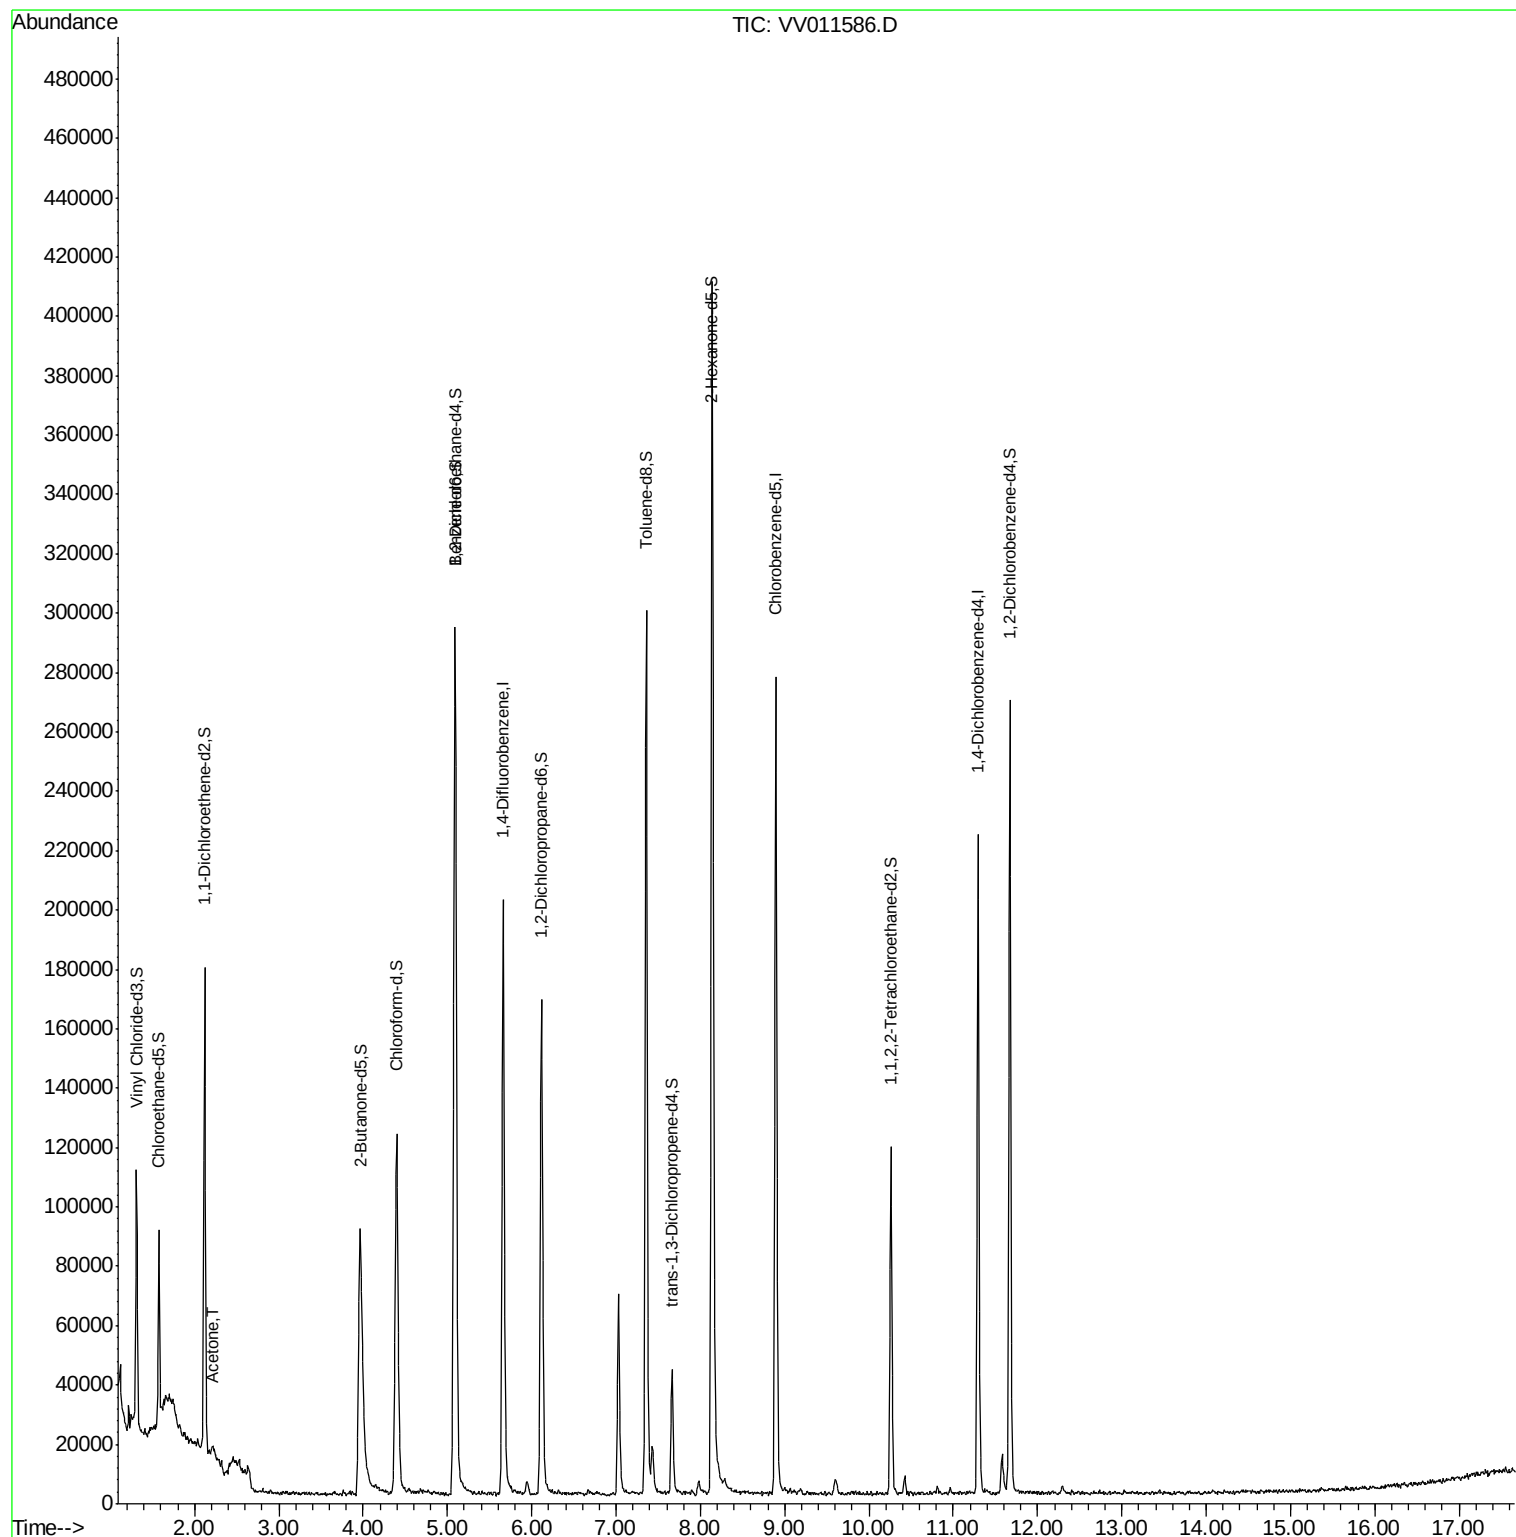

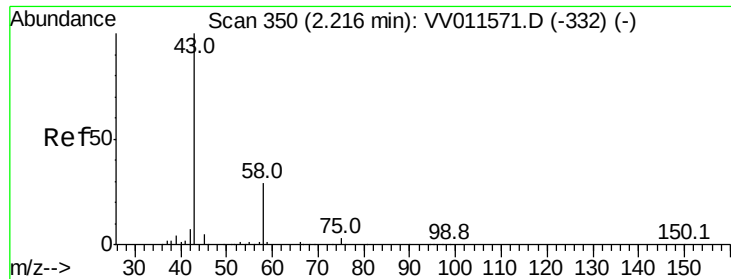

#13

Acetone

Concen: 3.087 ug/L

RT: 2.22 min Scan# 352

Delta R.T. 0.01 min

Lab File: VV011586.D

Acq: 18 Jun 2019 20:20

Instrument :
MSVOA_V
ClientSampleId :
BFCS9

Tot Ion: 43 Resp: 6894

Ion Ratio Lower Upper

43 100

58 10.1 0.0 57.8

