

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061919\
 Data File : VV011587.D
 Acq On : 18 Jun 2019 20:46
 Operator : SY/MD
 Sample : K3381-10
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFC58

Quant Time: Jun 19 02:54:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 19 02:08:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	177090	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	162831	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	62583	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	42091	3.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.00%
7) Chloroethane-d5	1.58	69	35758	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.40%
11) 1,1-Dichloroethene-d2	2.12	63	72079	2.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.60%#
20) 2-Butanone-d5	3.96	46	188123	50.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.00%
24) Chloroform-d	4.40	84	110616	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
26) 1,2-Dichloroethane-d4	5.08	65	68663	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.09	84	218237	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	6.12	67	70293	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.36	98	179760	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	7.67	79	18307	3.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.40%
46) 2-Hexanone-d5	8.14	63	139666	47.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51972	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	61059	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%


Target Compounds					Ovalue
13) Acetone	2.23	43	6114	2.411 ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061919\
Data File : VV011587.D
Acq On : 18 Jun 2019 20:46
Operator : SY/MD
Sample : K3381-10
Misc : 25ML/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCS8

Quant Time: Jun 19 02:54:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 19 02:08:53 2019
Response via : Initial Calibration

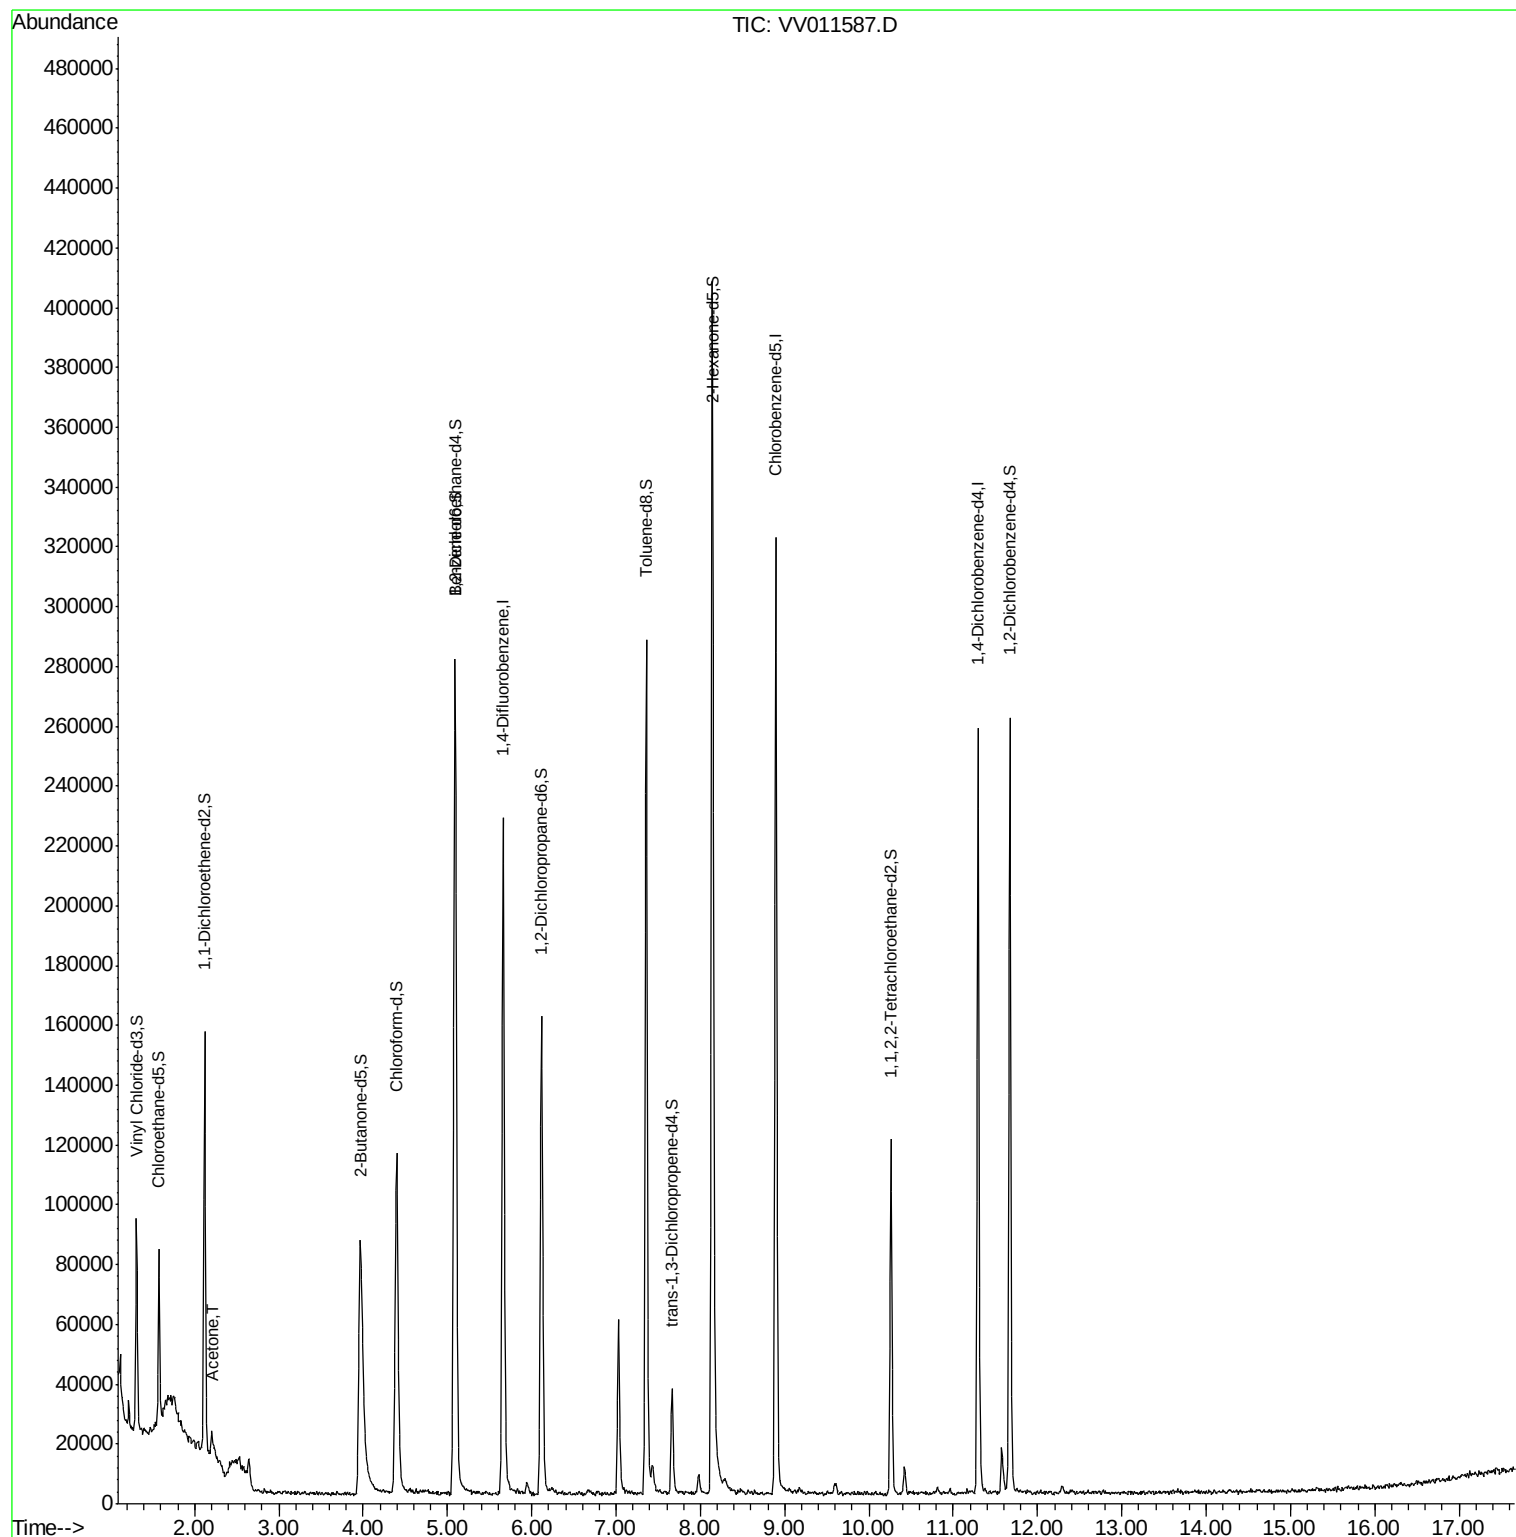

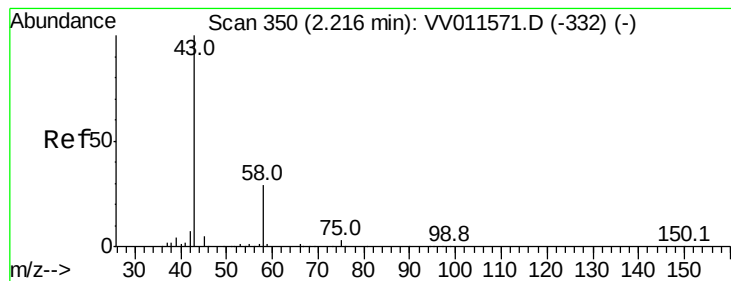

#13

Acetone

Concen: 2.411 ug/L

RT: 2.23 min Scan# 353

Delta R.T. 0.01 min

Lab File: VV011587.D

Acq: 18 Jun 2019 20:46

Instrument :
MSVOA_V
ClientSampleId :
BFCS8

Tot Ion: 43 Resp: 6114

Ion Ratio Lower Upper

43 100

58 16.5 0.0 57.8

