

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061919\
 Data File : VV011600.D
 Acq On : 19 Jun 2019 03:18
 Operator : SY/MD
 Sample : K3386-13
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM94

Quant Time: Jun 19 08:56:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 19 07:50:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	165981	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	150998	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	56034	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	37822	3.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	60.40%
7) Chloroethane-d5	1.58	69	32535	4.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.00%
11) 1,1-Dichloroethene-d2	2.12	63	63946	2.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.60%#
20) 2-Butanone-d5	3.96	46	198194	56.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.40%
24) Chloroform-d	4.40	84	107196	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.08	65	69042	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
32) Benzene-d6	5.09	84	204381	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
36) 1,2-Dichloropropane-d6	6.12	67	70433	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.36	98	160675	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.00%
43) trans-1,3-Dichloropropene-	7.67	79	17328	3.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.80%
46) 2-Hexanone-d5	8.14	63	143528	52.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.54%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	53532	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	56633	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%


Target Compounds					Ovalue
13) Acetone	2.23	43	7003	2.947 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061919\
Data File : VV011600.D
Acq On : 19 Jun 2019 03:18
Operator : SY/MD
Sample : K3386-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0M94

Quant Time: Jun 19 08:56:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 19 07:50:26 2019
Response via : Initial Calibration

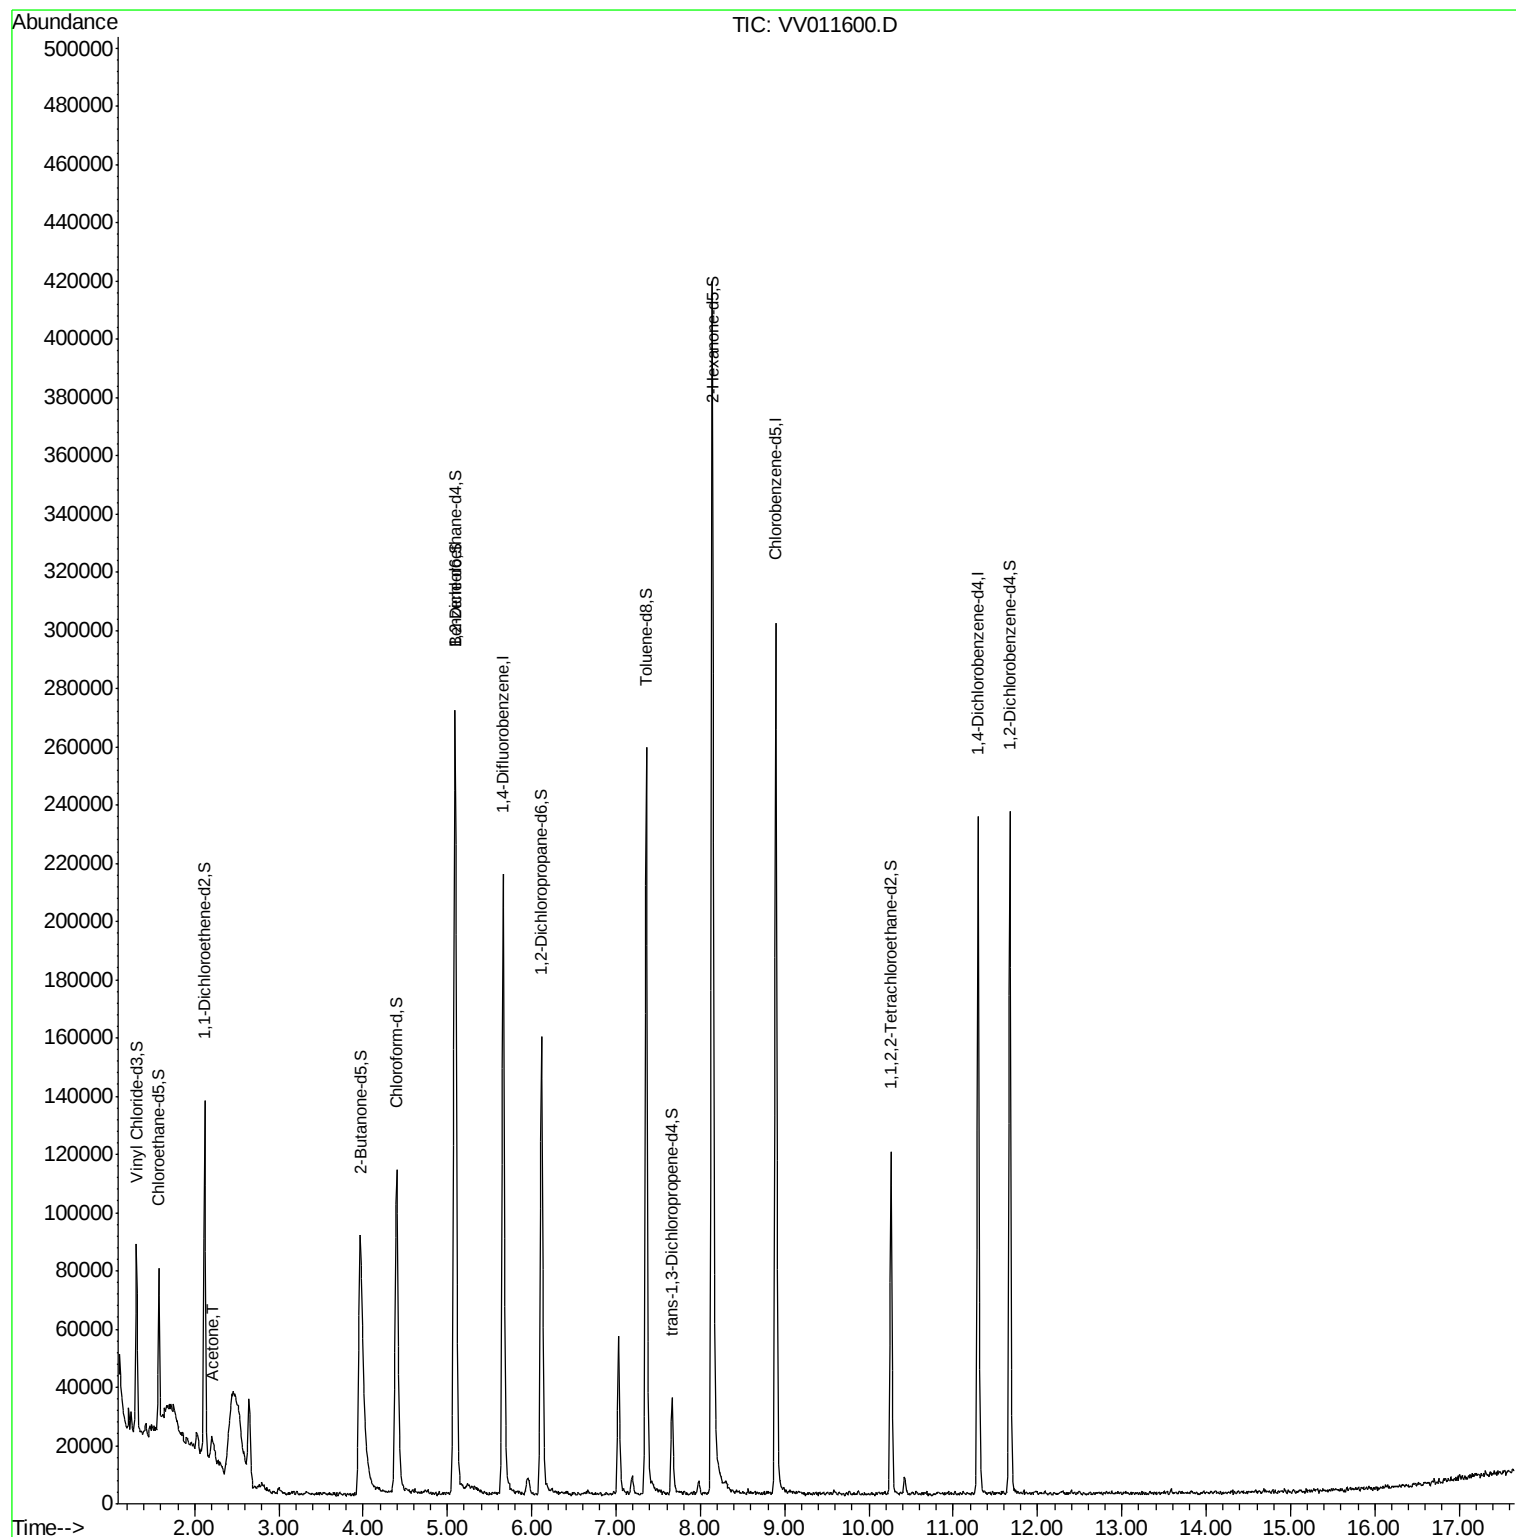

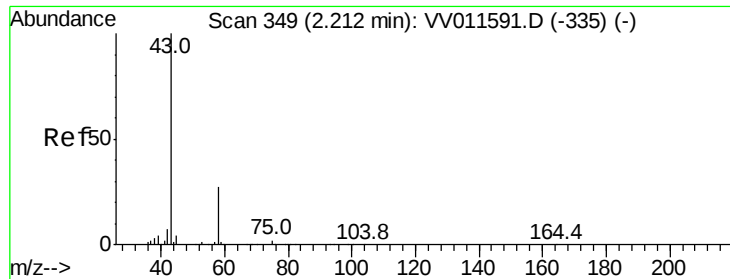

#13

Acetone

Concen: 2.947 ug/L

RT: 2.23 min Scan# 353

Delta R.T. 0.01 min

Lab File: VV011600.D

Acq: 19 Jun 2019 03:18

Instrument :
MSVOA_V
ClientSampleId :
COM94

Tot Ion: 43 Resp: 7003

Ion Ratio Lower Upper

43 100

58 20.9 0.0 57.8

