


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061919\
 Data File : VV011570.D
 Acq On : 18 Jun 2019 12:48
 Operator : SY/MD
 Sample : BFB51
 Misc : 25ML/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB51

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 19 02:08:53 2019

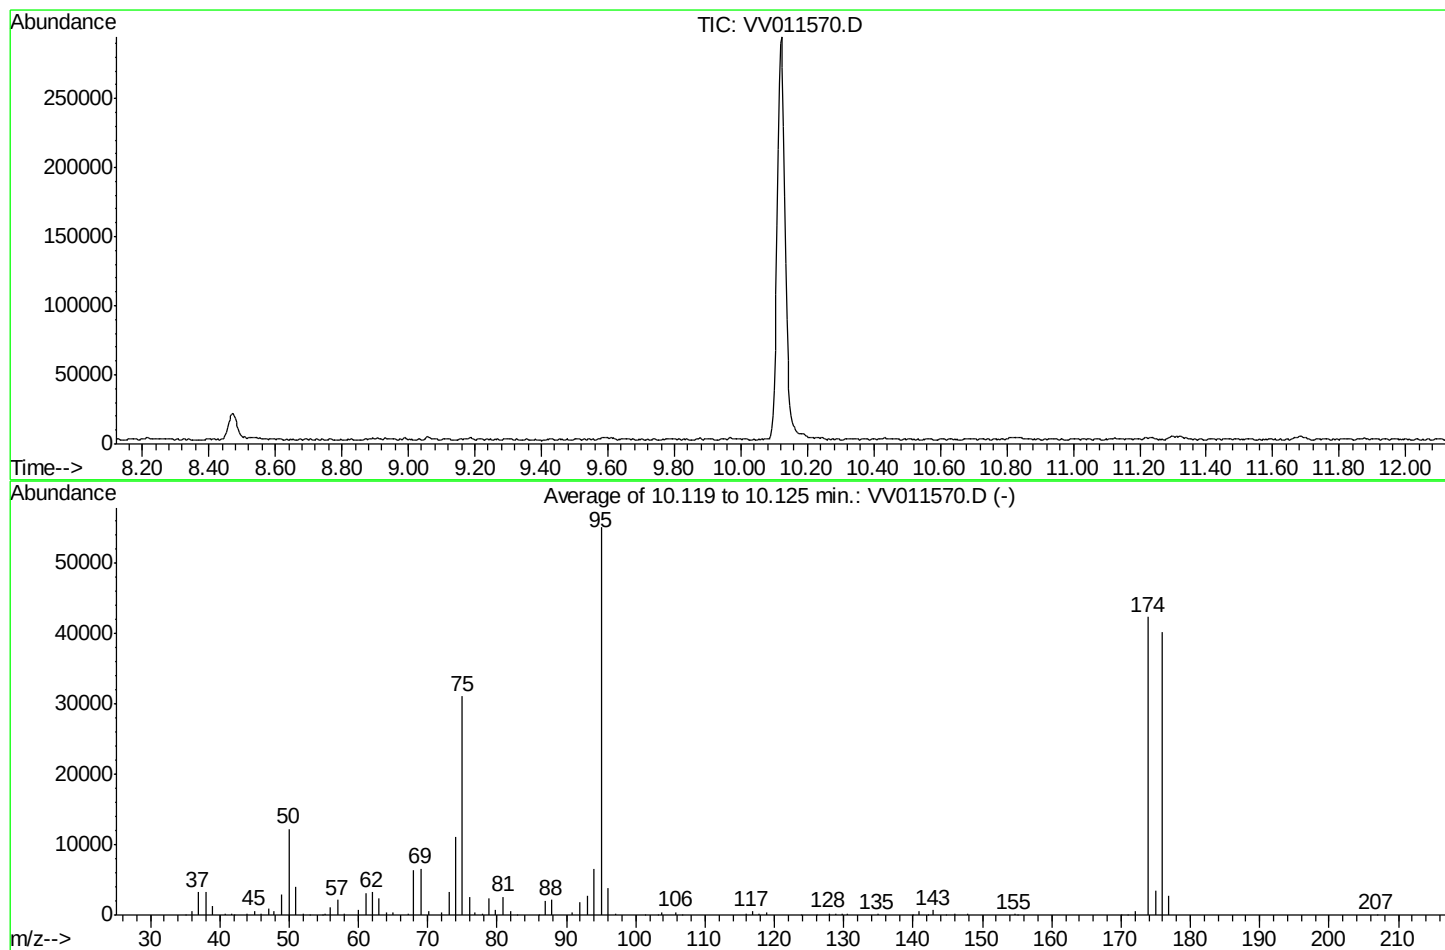

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	12235	PASS
75	95	30	80	56.3	31034	PASS
95	95	100	100	100.0	55088	PASS
96	95	5	9	6.8	3770	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.9	42336	PASS
175	174	5	9	8.1	3445	PASS
176	174	95	101	95.1	40266	PASS
177	176	5	9	6.6	2659	PASS

m/z	Abundance
35.90	168.0
36.90	142.0
39.90	1717.0
41.10	120.0
42.50	118.0
43.20	144.0
43.90	579.0
47.60	131.0
48.20	112.0
49.90	122.0
51.00	104.0
52.50	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.20	129.0
35.90	691.0
37.00	3504.0
38.00	3275.0
38.90	1363.0
39.90	1752.0
40.80	163.0
41.80	203.0
43.10	148.0
43.90	825.0
44.90	640.0
45.90	138.0
47.00	867.0
47.80	545.0
49.00	2895.0
50.00	12514.0
51.00	4299.0
52.00	206.0
54.90	229.0
55.90	1055.0
57.00	2337.0
58.10	144.0
60.00	674.0
61.00	3222.0
62.00	3169.0
63.00	2523.0
64.00	336.0
65.00	294.0
67.10	233.0
68.00	6687.0
69.00	6532.0
70.00	613.0
71.90	430.0
73.00	3263.0
74.00	11329.0
75.00	31728.0
76.00	2604.0
76.90	352.0
78.90	2375.0
79.80	775.0
80.90	2720.0
81.90	636.0
82.90	105.0
86.10	154.0
86.90	2084.0
87.90	2115.0
90.80	338.0
91.90	1993.0
93.00	2789.0
93.90	6742.0
95.00	55952.0
96.00	3832.0
97.00	183.0
103.10	104.0
103.70	335.0
105.80	395.0
106.70	126.0
115.90	288.0
116.80	501.0
117.70	271.0
118.80	427.0
123.80	100.0
126.00	102.0
127.80	309.0
128.80	117.0
129.80	190.0
130.60	103.0
134.80	177.0
140.00	119.0
140.90	642.0
142.10	111.0
142.90	752.0
144.70	109.0
146.00	122.0
147.90	211.0
154.70	173.0
172.00	570.0
173.90	42744.0
174.90	3611.0
175.90	39872.0
176.90	2689.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.10	106.0
36.00	726.0
36.90	3453.0
38.00	3366.0
38.90	1365.0
39.90	1682.0
40.80	154.0
41.70	189.0
43.00	126.0
43.90	782.0
45.00	667.0
46.00	131.0
47.00	1017.0
47.80	582.0
49.00	2949.0
50.00	12771.0
51.00	4167.0
52.00	206.0
53.00	126.0
55.10	218.0
56.00	1100.0
57.00	2176.0
58.00	127.0
60.00	670.0
61.00	3175.0
61.90	3306.0
63.00	2469.0
64.00	307.0
65.10	335.0
67.10	284.0
67.90	6513.0
69.00	6780.0
70.00	583.0
71.90	411.0
73.00	3379.0
74.00	11414.0
75.00	32032.0
76.00	2647.0
76.90	432.0
77.90	149.0
78.90	2322.0
79.80	725.0
80.90	2721.0
81.90	613.0
86.90	2138.0
87.90	2252.0
90.80	344.0
91.90	1966.0
93.00	2843.0
94.00	6717.0
95.00	56720.0
96.00	3918.0
97.00	167.0
103.10	103.0
103.70	362.0
105.80	403.0
106.70	104.0
115.80	283.0
116.80	513.0
117.70	275.0
118.80	410.0
126.00	106.0
127.80	277.0
128.80	152.0
129.80	203.0
130.60	135.0
134.80	179.0
140.00	123.0
140.90	610.0
142.20	137.0
142.90	740.0
144.60	107.0
146.00	112.0
147.80	198.0
154.60	164.0
170.00	103.0
171.00	113.0
171.90	605.0
173.90	43656.0
174.90	3564.0
175.90	41552.0
176.90	2736.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
36.00	698.0
36.90	3210.0
38.00	3086.0
38.90	1254.0
39.90	1668.0
40.80	140.0
41.80	154.0
42.10	146.0
43.10	109.0
44.00	733.0
45.00	608.0
45.90	108.0
47.00	899.0
47.90	549.0
49.00	2681.0
50.00	11787.0
51.00	3827.0
52.00	209.0
53.00	131.0
55.10	210.0
56.00	1180.0
57.00	1782.0
57.90	140.0
59.90	622.0
61.00	2898.0
61.90	3100.0
63.00	2176.0
64.00	299.0
65.10	344.0
67.10	284.0
68.00	5730.0
69.00	6471.0
70.10	505.0
71.90	374.0
73.00	3149.0
74.00	10371.0
75.00	29344.0
76.00	2386.0
76.80	456.0
77.90	168.0
78.90	2176.0
79.80	677.0
80.80	2389.0
81.90	571.0
86.90	2038.0
87.80	2116.0
90.80	307.0
91.90	1721.0
93.00	2655.0
94.00	6154.0
95.00	52592.0
96.00	3560.0
97.00	151.0
101.40	103.0
103.70	320.0
105.80	396.0
115.80	254.0
116.80	497.0
117.70	244.0
118.90	363.0
127.90	228.0
128.80	148.0
129.80	226.0
130.50	126.0
134.90	151.0
140.90	557.0
143.00	681.0
145.90	108.0
147.80	154.0
154.60	121.0
155.00	133.0
170.90	123.0
171.90	504.0
173.90	40608.0
174.90	3160.0
175.90	39376.0
176.90	2554.0
206.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51