

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017001.D
 Acq On : 19 Jun 2020 15:27
 Operator : SY/MD
 Sample : L3074-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	90	rVB	3034404	3127886	2.49%	1.152%
2	1.576	145	151	168	rVB	128133	150412	0.12%	0.055%
3	2.122	312	321	342	rVB3	355954	586847	0.47%	0.216%
4	2.720	506	507	509	rBV2	1065	421	0.00%	0.000%
5	2.778	513	525	546	rVV2	343602	626490	0.50%	0.231%
6	2.929	570	572	573	rBV3	1115	350	0.00%	0.000%
7	2.990	588	591	593	rBV3	1073	638	0.00%	0.000%
8	3.151	639	641	644	rBV4	915	387	0.00%	0.000%
9	3.351	699	703	706	rBV6	1942	1759	0.00%	0.001%
10	3.473	739	741	742	rBV2	866	335	0.00%	0.000%
11	3.566	763	770	774	rBV6	1399	1613	0.00%	0.001%
12	3.585	774	776	777	rBV2	801	295	0.00%	0.000%
13	3.614	782	785	787	rBV3	1719	1226	0.00%	0.000%
14	3.659	796	799	800	rBV2	903	401	0.00%	0.000%
15	3.682	804	806	808	rBV	1153	501	0.00%	0.000%
16	3.724	818	819	820	rBV	673	216	0.00%	0.000%
17	3.740	822	824	827	rVB3	1765	1005	0.00%	0.000%
18	3.759	827	830	833	rBV4	552	466	0.00%	0.000%
19	3.826	848	851	852	rBV3	1108	645	0.00%	0.000%
20	3.839	853	855	858	rVV2	1372	868	0.00%	0.000%
21	3.942	863	887	934	rBV2	32089630	84826212	67.52%	31.242%
22	4.376	1011	1022	1044	rVB	240083	572604	0.46%	0.211%
23	4.823	1159	1161	1163	rBV3	1355	642	0.00%	0.000%
24	5.071	1221	1238	1272	rBV2	561872	1505698	1.20%	0.555%
25	5.357	1322	1327	1328	rBV4	1801	1526	0.00%	0.001%
26	5.556	1387	1389	1390	rBV2	1231	462	0.00%	0.000%
27	5.576	1393	1395	1396	rBV2	1330	480	0.00%	0.000%
28	5.640	1403	1415	1436	rBV2	428961	848563	0.68%	0.313%
29	5.859	1478	1483	1486	rBV7	2002	1839	0.00%	0.001%
30	5.942	1491	1509	1540	rBV	23253273	46416216	36.95%	17.095%
31	6.093	1547	1556	1579	rVB	331637	664953	0.53%	0.245%
32	6.579	1705	1707	1711	rBV3	1548	1141	0.00%	0.000%
33	6.759	1759	1763	1766	rBV6	1776	1542	0.00%	0.001%
34	6.791	1769	1773	1774	rBV3	1128	734	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017001.D
 Acq On : 19 Jun 2020 15:27
 Operator : SY/MD
 Sample : L3074-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.865	1793	1796	1798	rVB4	1244	614	0.00%	0.000%
36	7.006	1829	1840	1859	rBV	194806	347896	0.28%	0.128%
37	7.338	1931	1943	1957	rBV	690940	1178266	0.94%	0.434%
38	7.643	2028	2038	2059	rVB	135912	231379	0.18%	0.085%
39	7.801	2085	2087	2091	rBV3	1905	1117	0.00%	0.000%
40	7.846	2097	2101	2103	rBV3	1412	1021	0.00%	0.000%
41	7.900	2115	2118	2120	rBV3	1124	807	0.00%	0.000%
42	8.019	2133	2155	2174	rBV	61583591	125625213	100.00%	46.268%
43	8.106	2176	2182	2218	rVB	402964	733570	0.58%	0.270%
44	8.874	2410	2421	2444	rBV	653844	1086873	0.87%	0.400%
45	9.128	2495	2500	2503	rBV7	2287	2290	0.00%	0.001%
46	9.164	2504	2511	2524	rVB3	17224	30781	0.02%	0.011%
47	9.395	2580	2583	2586	rVB4	1811	1233	0.00%	0.000%
48	9.566	2632	2636	2648	rVB7	7097	10205	0.01%	0.004%
49	9.672	2665	2669	2673	rBV7	1478	1290	0.00%	0.000%
50	9.707	2678	2680	2685	rBV6	1538	1268	0.00%	0.000%
51	9.746	2690	2692	2693	rBV2	803	312	0.00%	0.000%
52	9.820	2713	2715	2716	rBV2	1327	578	0.00%	0.000%
53	9.897	2733	2739	2742	rBV6	2168	2129	0.00%	0.001%
54	10.238	2832	2845	2860	rBV	422101	664349	0.53%	0.245%
55	10.463	2913	2915	2916	rBV3	1309	454	0.00%	0.000%
56	10.630	2965	2967	2970	rBV2	1175	538	0.00%	0.000%
57	10.678	2978	2982	2986	rBV5	1594	1567	0.00%	0.001%
58	10.833	3026	3030	3032	rBV4	1197	962	0.00%	0.000%
59	10.929	3058	3060	3061	rBV3	1968	750	0.00%	0.000%
60	11.019	3086	3088	3091	rBV3	1719	1300	0.00%	0.000%
61	11.093	3108	3111	3112	rBV3	2048	1274	0.00%	0.000%
62	11.270	3155	3166	3184	rBV	704715	1080740	0.86%	0.398%
63	11.646	3269	3283	3298	rBV	738369	1144277	0.91%	0.421%
64	11.884	3355	3357	3360	rBV2	846	449	0.00%	0.000%
65	11.977	3384	3386	3388	rBV2	1330	815	0.00%	0.000%
66	12.096	3421	3423	3425	rBV2	996	460	0.00%	0.000%
67	12.157	3440	3442	3443	rBV2	952	463	0.00%	0.000%
68	12.263	3473	3475	3480	rBV6	2201	1495	0.00%	0.001%
69	12.466	3535	3538	3539	rBV2	813	491	0.00%	0.000%
70	12.514	3551	3553	3557	rBV4	1133	827	0.00%	0.000%
71	12.733	3619	3621	3624	rBV4	1284	660	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017001.D
 Acq On : 19 Jun 2020 15:27
 Operator : SY/MD
 Sample : L3074-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.759	3624	3629	3634	rBV7	1852	2525	0.00%	0.001%
73	12.807	3640	3644	3646	rBV4	1172	861	0.00%	0.000%
74	12.836	3650	3653	3654	rBV3	872	512	0.00%	0.000%
75	12.871	3662	3664	3666	rBV3	1237	564	0.00%	0.000%
76	12.884	3666	3668	3669	rBV2	633	197	0.00%	0.000%
77	13.083	3728	3730	3732	rBV3	1274	552	0.00%	0.000%
78	13.160	3751	3754	3757	rBV5	1025	807	0.00%	0.000%
79	13.254	3781	3783	3787	rBV4	1355	932	0.00%	0.000%
80	13.357	3812	3815	3818	rBV3	1334	943	0.00%	0.000%
81	13.418	3832	3834	3837	rBV2	1234	577	0.00%	0.000%
82	13.443	3840	3842	3843	rBV2	1151	434	0.00%	0.000%
83	13.791	3947	3950	3952	rBV3	1545	1101	0.00%	0.000%
84	13.877	3975	3977	3978	rBV2	788	255	0.00%	0.000%
85	14.524	4175	4178	4179	rBV2	1236	492	0.00%	0.000%
86	14.546	4183	4185	4187	rBV3	1709	788	0.00%	0.000%
87	14.758	4248	4251	4253	rBV4	1305	695	0.00%	0.000%
88	15.122	4362	4364	4365	rBV2	994	494	0.00%	0.000%


Sum of corrected areas: 271516815

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
Data File : VV017001.D
Acq On : 19 Jun 2020 15:27
Operator : SY/MD
Sample : L3074-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M04

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

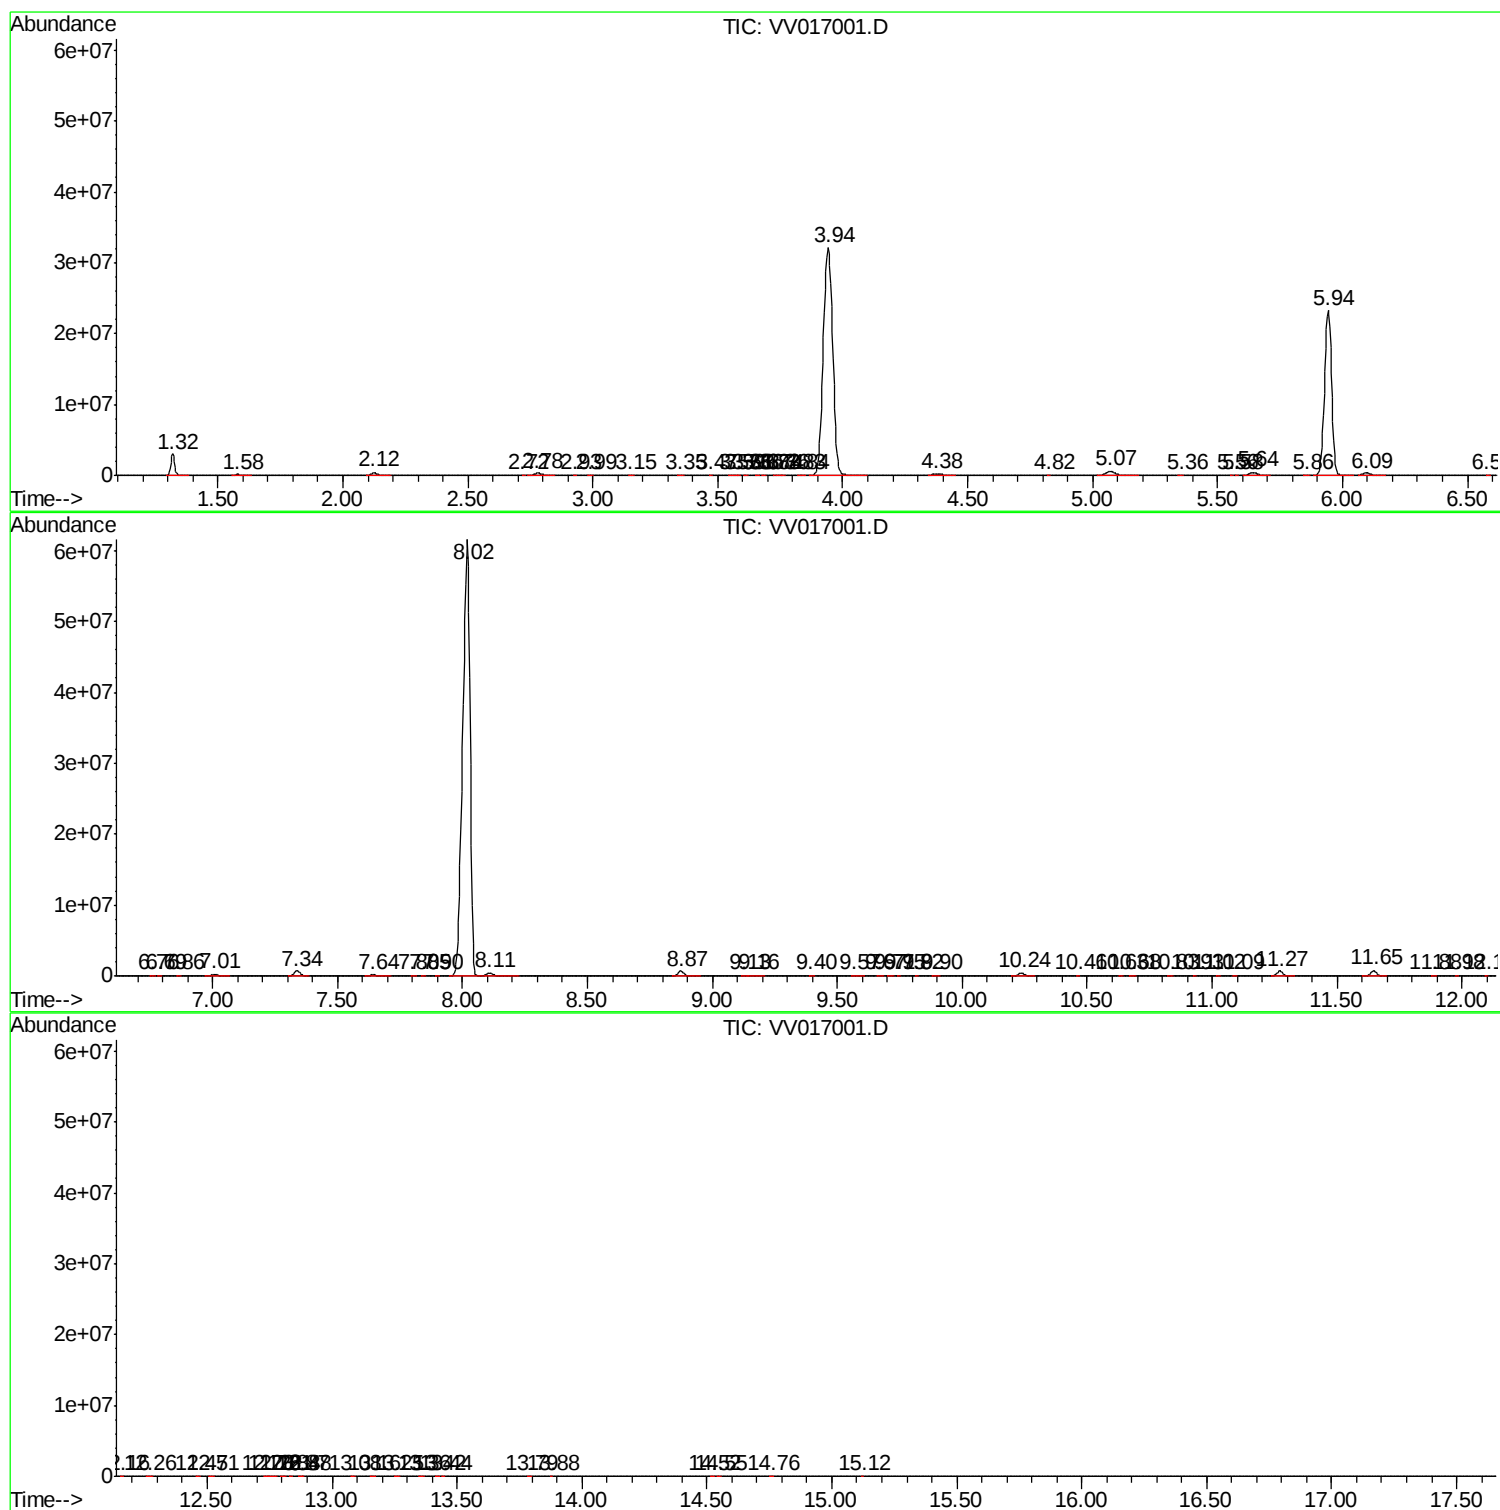

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017001.D
Acq On : 19 Jun 2020 15:27
Operator : SY/MD
Sample : L3074-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M04

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017001.D
Acq On : 19 Jun 2020 15:27
Operator : SY/MD
Sample : L3074-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M04

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
