

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017002.D
 Acq On : 19 Jun 2020 15:50
 Operator : SY/MD
 Sample : L3074-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	79	rBV	179521	179654	12.49%	1.496%
2	1.579	146	152	161	rVB	122276	131283	9.12%	1.093%
3	2.122	310	321	336	rBV	289202	439076	30.52%	3.655%
4	2.621	474	476	480	rVB2	1789	796	0.06%	0.007%
5	2.907	562	565	568	rBV4	1197	826	0.06%	0.007%
6	2.984	587	589	593	rBV4	1022	585	0.04%	0.005%
7	3.003	593	595	600	rVB4	1613	1256	0.09%	0.010%
8	3.029	600	603	606	rBV5	1080	711	0.05%	0.006%
9	3.148	634	640	643	rBV6	1439	1654	0.11%	0.014%
10	3.167	644	646	649	rVV3	1212	840	0.06%	0.007%
11	3.196	653	655	657	rVV2	1206	493	0.03%	0.004%
12	3.376	708	711	713	rVB4	1661	811	0.06%	0.007%
13	3.389	713	715	719	rBV4	1021	929	0.06%	0.008%
14	3.511	748	753	757	rVV8	1245	1490	0.10%	0.012%
15	3.646	790	795	798	rBV6	1375	1345	0.09%	0.011%
16	3.839	849	855	858	rBV8	1706	2063	0.14%	0.017%
17	3.936	861	885	908	rBV2	156489	576175	40.05%	4.797%
18	4.277	988	991	994	rBV4	1643	1480	0.10%	0.012%
19	4.376	1008	1022	1049	rVB	223046	544051	37.81%	4.529%
20	4.634	1100	1102	1105	rVB3	1314	641	0.04%	0.005%
21	4.653	1105	1108	1110	rBV4	1408	905	0.06%	0.008%
22	4.785	1146	1149	1151	rBV3	1342	939	0.07%	0.008%
23	4.817	1155	1159	1162	rBV5	1136	929	0.06%	0.008%
24	4.926	1191	1193	1197	rBV5	954	757	0.05%	0.006%
25	5.071	1221	1238	1266	rBV2	532240	1370437	95.25%	11.409%
26	5.502	1370	1372	1374	rBV2	1319	607	0.04%	0.005%
27	5.563	1389	1391	1393	rBV4	1622	751	0.05%	0.006%
28	5.640	1403	1415	1440	rVV	387394	769699	53.50%	6.408%
29	5.810	1466	1468	1471	rBV4	996	729	0.05%	0.006%
30	5.939	1497	1508	1525	rVB4	106249	221727	15.41%	1.846%
31	6.093	1544	1556	1580	rVB	308629	609349	42.35%	5.073%
32	6.392	1647	1649	1650	rBV	1657	542	0.04%	0.005%
33	6.444	1661	1665	1667	rBV5	1930	1922	0.13%	0.016%
34	6.508	1683	1685	1686	rBV2	1110	496	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017002.D
 Acq On : 19 Jun 2020 15:50
 Operator : SY/MD
 Sample : L3074-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.720	1748	1751	1754	rBV5	2298	1529	0.11%	0.013%
36	6.862	1793	1795	1800	rVB5	1720	1199	0.08%	0.010%
37	6.900	1802	1807	1811	rBV7	1885	1505	0.10%	0.013%
38	7.006	1828	1840	1868	rBV	175406	325917	22.65%	2.713%
39	7.183	1894	1895	1899	rBV3	1123	775	0.05%	0.006%
40	7.338	1931	1943	1964	rBV	643234	1092658	75.95%	9.096%
41	7.643	2028	2038	2057	rBV	125448	211210	14.68%	1.758%
42	7.897	2112	2117	2119	rBV4	2195	1602	0.11%	0.013%
43	7.936	2125	2129	2130	rBV4	1465	791	0.05%	0.007%
44	7.945	2130	2132	2135	rVV3	2216	1406	0.10%	0.012%
45	7.997	2135	2148	2168	rVV	859086	1438742	100.00%	11.978%
46	8.109	2173	2183	2217	rVV	305136	574307	39.92%	4.781%
47	8.402	2272	2274	2276	rBV3	1622	726	0.05%	0.006%
48	8.550	2319	2320	2323	rBV3	917	552	0.04%	0.005%
49	8.640	2345	2348	2351	rBV5	1261	1004	0.07%	0.008%
50	8.875	2409	2421	2441	rVV	577342	928596	64.54%	7.731%
51	9.112	2492	2495	2496	rBV2	1284	796	0.06%	0.007%
52	9.164	2507	2511	2515	rBV6	1642	1752	0.12%	0.015%
53	9.299	2550	2553	2554	rBV3	1218	635	0.04%	0.005%
54	9.344	2565	2567	2572	rVB6	1456	804	0.06%	0.007%
55	9.373	2572	2576	2578	rBV4	1044	830	0.06%	0.007%
56	9.601	2644	2647	2649	rBV2	1092	706	0.05%	0.006%
57	9.717	2678	2683	2689	rBV9	2063	2943	0.20%	0.025%
58	9.768	2692	2699	2700	rBV5	1325	1294	0.09%	0.011%
59	9.862	2725	2728	2730	rBV3	1459	1050	0.07%	0.009%
60	9.929	2746	2749	2751	rBV3	1296	727	0.05%	0.006%
61	9.965	2758	2760	2763	rVV3	1010	480	0.03%	0.004%
62	10.238	2833	2845	2858	rBV	376789	591502	41.11%	4.924%
63	10.383	2887	2890	2891	rBV3	1062	626	0.04%	0.005%
64	10.392	2891	2893	2896	rVV4	2162	1508	0.10%	0.013%
65	10.765	3004	3009	3012	rBV5	1356	1456	0.10%	0.012%
66	10.829	3026	3029	3035	rBV8	1447	1329	0.09%	0.011%
67	10.865	3038	3040	3042	rBV2	942	660	0.05%	0.005%
68	10.897	3049	3050	3054	rBV3	1156	635	0.04%	0.005%
69	11.055	3097	3099	3108	rVB8	1665	1567	0.11%	0.013%
70	11.148	3125	3128	3130	rBV3	989	768	0.05%	0.006%
71	11.270	3154	3166	3186	rBV	575783	890247	61.88%	7.411%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017002.D
 Acq On : 19 Jun 2020 15:50
 Operator : SY/MD
 Sample : L3074-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3301	rBV	673906	1034208	71.88%	8.610%
73	11.855	3346	3348	3353	rVB6	1557	1133	0.08%	0.009%
74	11.894	3357	3360	3366	rVB6	1411	1174	0.08%	0.010%
75	11.929	3366	3371	3374	rVB7	1729	1459	0.10%	0.012%
76	11.997	3390	3392	3394	rBV2	1402	777	0.05%	0.006%
77	12.087	3417	3420	3421	rBV2	1057	542	0.04%	0.005%
78	12.244	3465	3469	3470	rBV4	964	656	0.05%	0.005%
79	12.434	3525	3528	3530	rBV3	1278	677	0.05%	0.006%
80	12.453	3530	3534	3538	rBV7	2228	2080	0.14%	0.017%
81	12.624	3585	3587	3588	rBV2	897	455	0.03%	0.004%
82	12.759	3625	3629	3631	rVB5	2141	1248	0.09%	0.010%
83	12.903	3671	3674	3675	rBV2	1815	883	0.06%	0.007%
84	13.022	3708	3711	3714	rBV4	1037	733	0.05%	0.006%
85	13.286	3791	3793	3799	rBV6	1637	1809	0.13%	0.015%
86	13.392	3823	3826	3828	rBV4	1065	769	0.05%	0.006%
87	13.431	3836	3838	3842	rBV4	1272	808	0.06%	0.007%
88	13.469	3848	3850	3852	rBV3	967	595	0.04%	0.005%
89	13.598	3886	3890	3891	rBV4	1271	915	0.06%	0.008%
90	13.624	3896	3898	3900	rBV3	1365	778	0.05%	0.006%
91	13.752	3936	3938	3942	rBV4	1035	763	0.05%	0.006%
92	13.784	3944	3948	3950	rBV4	1120	1063	0.07%	0.009%
93	13.874	3973	3976	3978	rBV3	1658	1153	0.08%	0.010%
94	13.919	3987	3990	3992	rBV3	1082	886	0.06%	0.007%
95	14.038	4025	4027	4030	rBV4	1180	893	0.06%	0.007%
96	14.099	4042	4046	4050	rBV6	1665	1778	0.12%	0.015%
97	14.177	4068	4070	4074	rVB2	1435	714	0.05%	0.006%
98	14.273	4097	4100	4101	rBV3	1302	628	0.04%	0.005%
99	14.903	4293	4296	4297	rBV3	1831	1046	0.07%	0.009%
100	15.341	4430	4432	4433	rBV2	1727	629	0.04%	0.005%


Sum of corrected areas: 12012034

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061920\
Data File : VV017002.D
Acq On : 19 Jun 2020 15:50
Operator : SY/MD
Sample : L3074-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9M05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

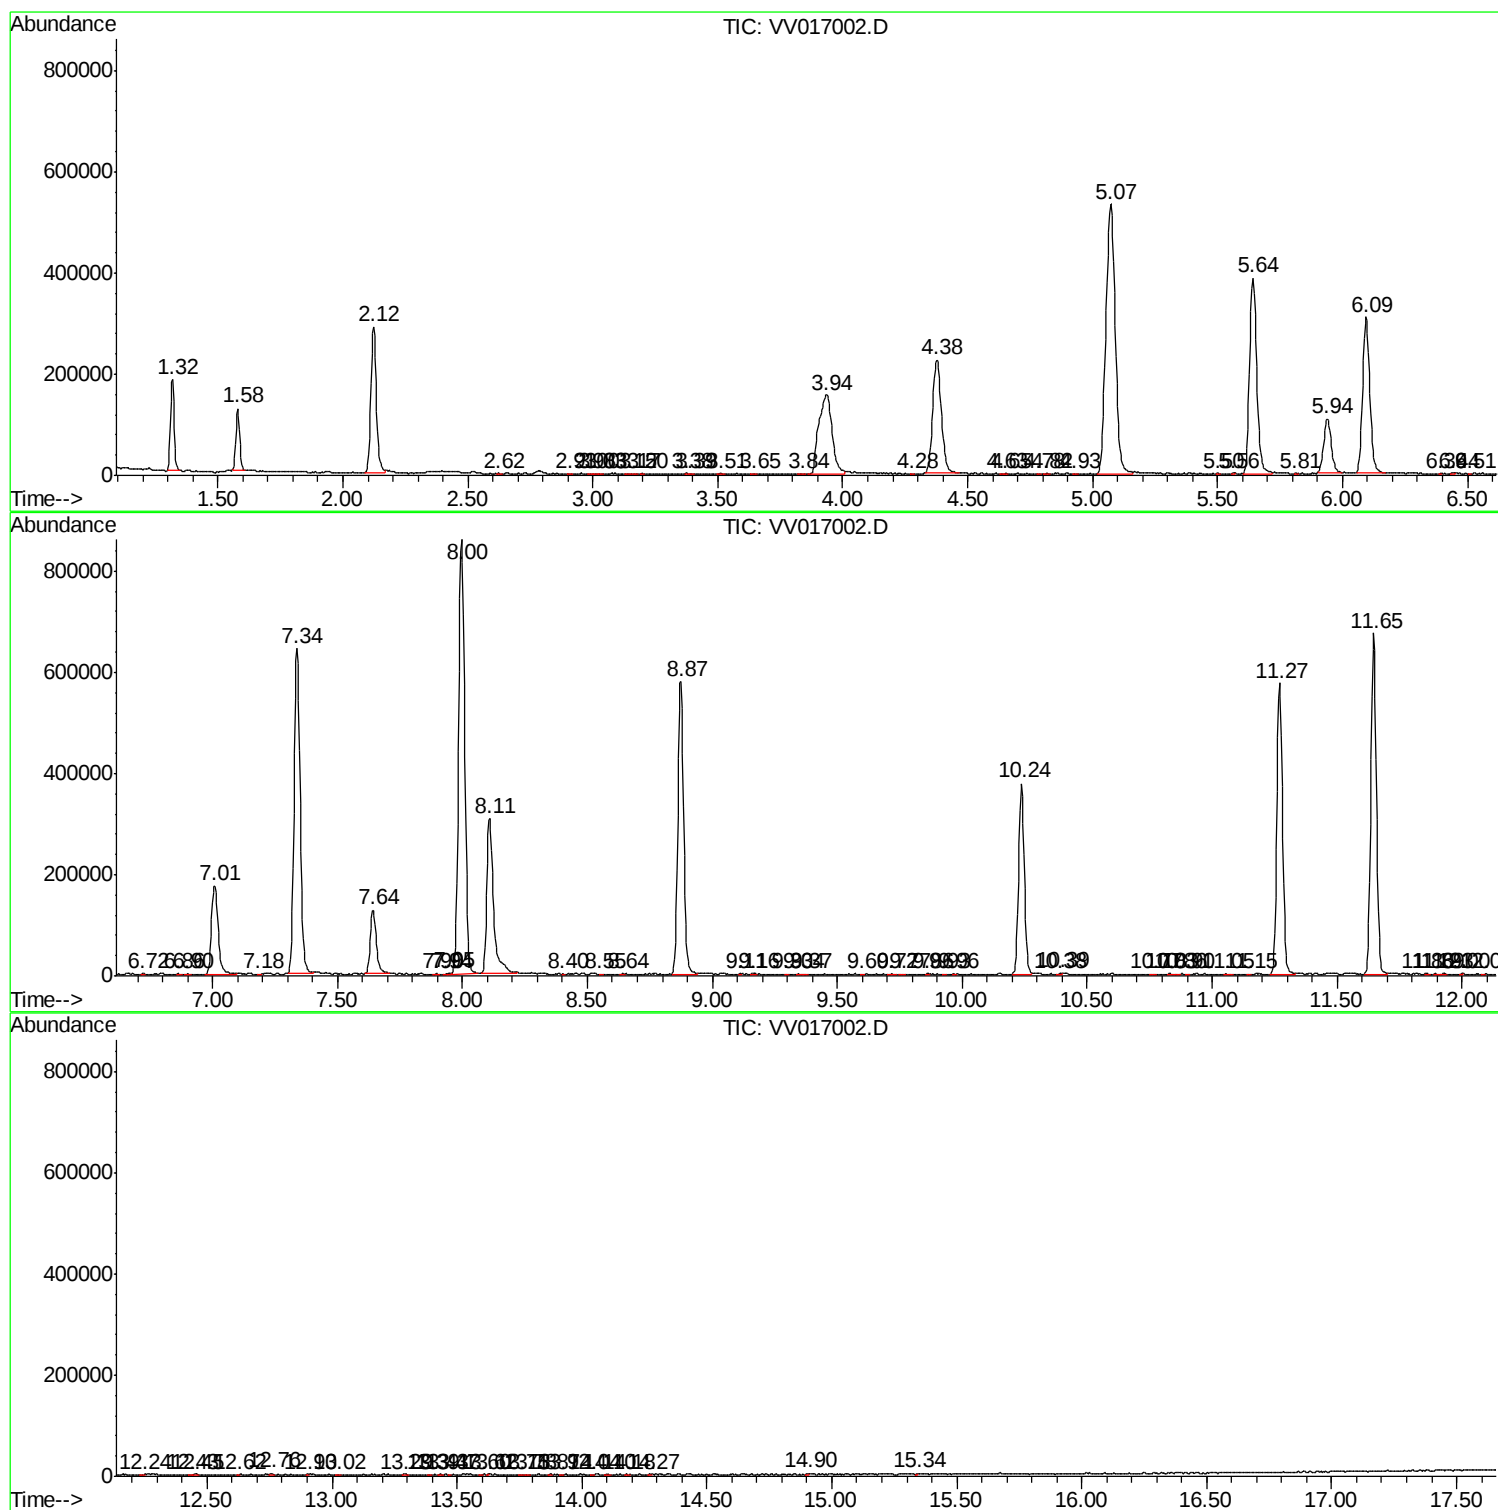

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017002.D
Acq On : 19 Jun 2020 15:50
Operator : SY/MD
Sample : L3074-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M05

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017002.D
Acq On : 19 Jun 2020 15:50
Operator : SY/MD
Sample : L3074-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M05

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc