

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061920\
 Data File : VV017003.D
 Acq On : 19 Jun 2020 16:39
 Operator : SY/MD
 Sample : VIBLK60
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	172049	175368	12.99%	1.746%
2	1.579	145	152	162	rBV	121989	134302	9.94%	1.337%
3	2.119	311	320	343	rVB	277907	421555	31.21%	4.197%
4	2.457	419	425	428	rBV7	2037	2114	0.16%	0.021%
5	2.569	457	460	463	rBV5	1488	1383	0.10%	0.014%
6	2.708	499	503	504	rBV4	1352	911	0.07%	0.009%
7	2.865	548	552	557	rVB6	1723	1408	0.10%	0.014%
8	2.891	557	560	561	rBV3	1529	708	0.05%	0.007%
9	2.942	573	576	579	rBV4	1064	827	0.06%	0.008%
10	2.968	582	584	590	rBV7	1731	1679	0.12%	0.017%
11	3.110	625	628	631	rBV4	1728	1163	0.09%	0.012%
12	3.405	718	720	724	rBV6	1101	940	0.07%	0.009%
13	3.438	728	730	734	rVV5	1459	1056	0.08%	0.011%
14	3.470	737	740	743	rVV4	1017	810	0.06%	0.008%
15	3.537	757	761	764	rBV5	1532	1143	0.08%	0.011%
16	3.704	810	813	814	rBV4	1000	539	0.04%	0.005%
17	3.733	819	822	825	rBV3	1232	806	0.06%	0.008%
18	3.769	831	833	836	rVB3	1381	686	0.05%	0.007%
19	3.823	848	850	854	rVB4	1737	1124	0.08%	0.011%
20	3.849	854	858	860	rBV3	1378	1228	0.09%	0.012%
21	3.910	866	877	905	rBV	90378	278227	20.60%	2.770%
22	4.373	1006	1021	1044	rBV	219979	539172	39.92%	5.368%
23	4.856	1169	1171	1172	rBV	1096	543	0.04%	0.005%
24	5.071	1220	1238	1263	rVV2	522511	1350524	100.00%	13.446%
25	5.396	1337	1339	1342	rBV4	1598	944	0.07%	0.009%
26	5.463	1358	1360	1363	rBV3	1815	878	0.07%	0.009%
27	5.511	1373	1375	1379	rBV4	1170	861	0.06%	0.009%
28	5.640	1400	1415	1438	rBV	413871	821798	60.85%	8.182%
29	5.823	1468	1472	1475	rBV6	1786	1618	0.12%	0.016%
30	6.093	1541	1556	1577	rBV	300797	608899	45.09%	6.062%
31	6.428	1659	1660	1664	rVB3	1093	683	0.05%	0.007%
32	6.486	1675	1678	1685	rVB8	1804	1806	0.13%	0.018%
33	6.518	1685	1688	1690	rBV4	1791	980	0.07%	0.010%
34	6.730	1753	1754	1759	rVB4	1563	1033	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061920\
 Data File : VV017003.D
 Acq On : 19 Jun 2020 16:39
 Operator : SY/MD
 Sample : VIBLK60
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.759	1759	1763	1766	rBV5	2497	1802	0.13%	0.018%
36	6.881	1792	1801	1803	rBV7	1622	1882	0.14%	0.019%
37	6.923	1812	1814	1819	rVB4	1459	1204	0.09%	0.012%
38	7.007	1829	1840	1857	rBV	173385	311791	23.09%	3.104%
39	7.232	1908	1910	1912	rBV2	1400	555	0.04%	0.006%
40	7.338	1930	1943	1959	rBV	628982	1075849	79.66%	10.711%
41	7.566	2012	2014	2017	rBV2	1149	725	0.05%	0.007%
42	7.582	2017	2019	2024	rVV6	1225	1104	0.08%	0.011%
43	7.640	2028	2037	2053	rVV2	120267	207361	15.35%	2.065%
44	7.833	2095	2097	2102	rBV5	1297	1218	0.09%	0.012%
45	8.109	2172	2183	2217	rBV	287951	562901	41.68%	5.604%
46	8.376	2263	2266	2268	rBV3	1604	1131	0.08%	0.011%
47	8.502	2303	2305	2308	rBV4	1566	595	0.04%	0.006%
48	8.672	2352	2358	2360	rBV6	1570	1638	0.12%	0.016%
49	8.756	2381	2384	2385	rBV3	1160	540	0.04%	0.005%
50	8.817	2401	2403	2407	rVB4	1774	1289	0.10%	0.013%
51	8.871	2407	2420	2439	rBV	598512	974351	72.15%	9.701%
52	9.032	2465	2470	2473	rBV6	1962	2252	0.17%	0.022%
53	9.148	2503	2506	2508	rBV4	1209	802	0.06%	0.008%
54	9.161	2508	2510	2513	rBV5	1475	1011	0.07%	0.010%
55	9.254	2537	2539	2541	rVB3	1171	542	0.04%	0.005%
56	9.267	2541	2543	2547	rVB4	1108	653	0.05%	0.007%
57	9.315	2555	2558	2561	rVV4	1970	1227	0.09%	0.012%
58	9.344	2564	2567	2570	rBV3	1507	829	0.06%	0.008%
59	9.392	2580	2582	2587	rVB3	1601	1064	0.08%	0.011%
60	9.457	2600	2602	2605	rVB3	1619	950	0.07%	0.009%
61	9.762	2694	2697	2702	rVB6	1432	1143	0.08%	0.011%
62	9.952	2751	2756	2761	rBV6	2683	3568	0.26%	0.036%
63	10.132	2809	2812	2816	rVB4	1128	800	0.06%	0.008%
64	10.158	2816	2820	2824	rVB6	1619	1231	0.09%	0.012%
65	10.177	2824	2826	2830	rBV5	879	781	0.06%	0.008%
66	10.238	2832	2845	2859	rBV	353305	555499	41.13%	5.531%
67	10.444	2907	2909	2913	rBV5	919	591	0.04%	0.006%
68	10.527	2932	2935	2936	rBV	1459	662	0.05%	0.007%
69	10.807	3020	3022	3026	rBV5	1630	960	0.07%	0.010%
70	11.032	3089	3092	3093	rBV2	1418	690	0.05%	0.007%
71	11.122	3118	3120	3122	rBV3	1277	556	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061920\
 Data File : VV017003.D
 Acq On : 19 Jun 2020 16:39
 Operator : SY/MD
 Sample : VIBLK60
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3183	rBV	592245	901527	66.75%	8.976%
73	11.408	3205	3209	3210	rBV3	1204	759	0.06%	0.008%
74	11.553	3250	3254	3258	rBV6	1627	1745	0.13%	0.017%
75	11.646	3270	3283	3296	rBV	635915	994955	73.67%	9.906%
76	11.878	3353	3355	3358	rVB4	1432	730	0.05%	0.007%
77	12.003	3389	3394	3396	rBV5	1594	1331	0.10%	0.013%
78	12.080	3415	3418	3420	rBV3	1556	624	0.05%	0.006%
79	12.164	3442	3444	3447	rBV4	827	534	0.04%	0.005%
80	12.231	3461	3465	3468	rBV5	1554	1237	0.09%	0.012%
81	12.248	3468	3470	3473	rVV3	1186	508	0.04%	0.005%
82	12.276	3478	3479	3482	rVB3	1098	497	0.04%	0.005%
83	12.325	3492	3494	3497	rBV4	1317	800	0.06%	0.008%
84	12.540	3559	3561	3562	rBV2	1166	616	0.05%	0.006%
85	12.675	3592	3603	3611	rBV2	4484	8826	0.65%	0.088%
86	12.765	3627	3631	3632	rBV3	1030	677	0.05%	0.007%
87	12.804	3640	3643	3644	rBV2	885	524	0.04%	0.005%
88	12.997	3701	3703	3707	rBV3	1748	1156	0.09%	0.012%
89	13.106	3735	3737	3740	rBV3	911	655	0.05%	0.007%
90	13.141	3745	3748	3756	rVB10	2113	2217	0.16%	0.022%
91	13.286	3788	3793	3802	rBV10	5538	7700	0.57%	0.077%
92	13.527	3862	3868	3880	rBV2	8531	16832	1.25%	0.168%
93	13.720	3925	3928	3932	rBV4	1241	1211	0.09%	0.012%
94	13.772	3938	3944	3955	rVB4	6862	11387	0.84%	0.113%
95	14.013	4014	4019	4023	rBV6	2304	2385	0.18%	0.024%
96	14.447	4150	4154	4156	rBV4	1146	1065	0.08%	0.011%
97	14.492	4165	4168	4171	rBV5	1718	1117	0.08%	0.011%
98	14.694	4228	4231	4232	rBV3	1599	831	0.06%	0.008%
99	14.813	4267	4268	4271	rBV3	1256	569	0.04%	0.006%
100	15.280	4407	4413	4415	rBV7	1290	1394	0.10%	0.014%


Sum of corrected areas: 10043872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061920\
Data File : VV017003.D
Acq On : 19 Jun 2020 16:39
Operator : SY/MD
Sample : VIBLK60
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK60

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

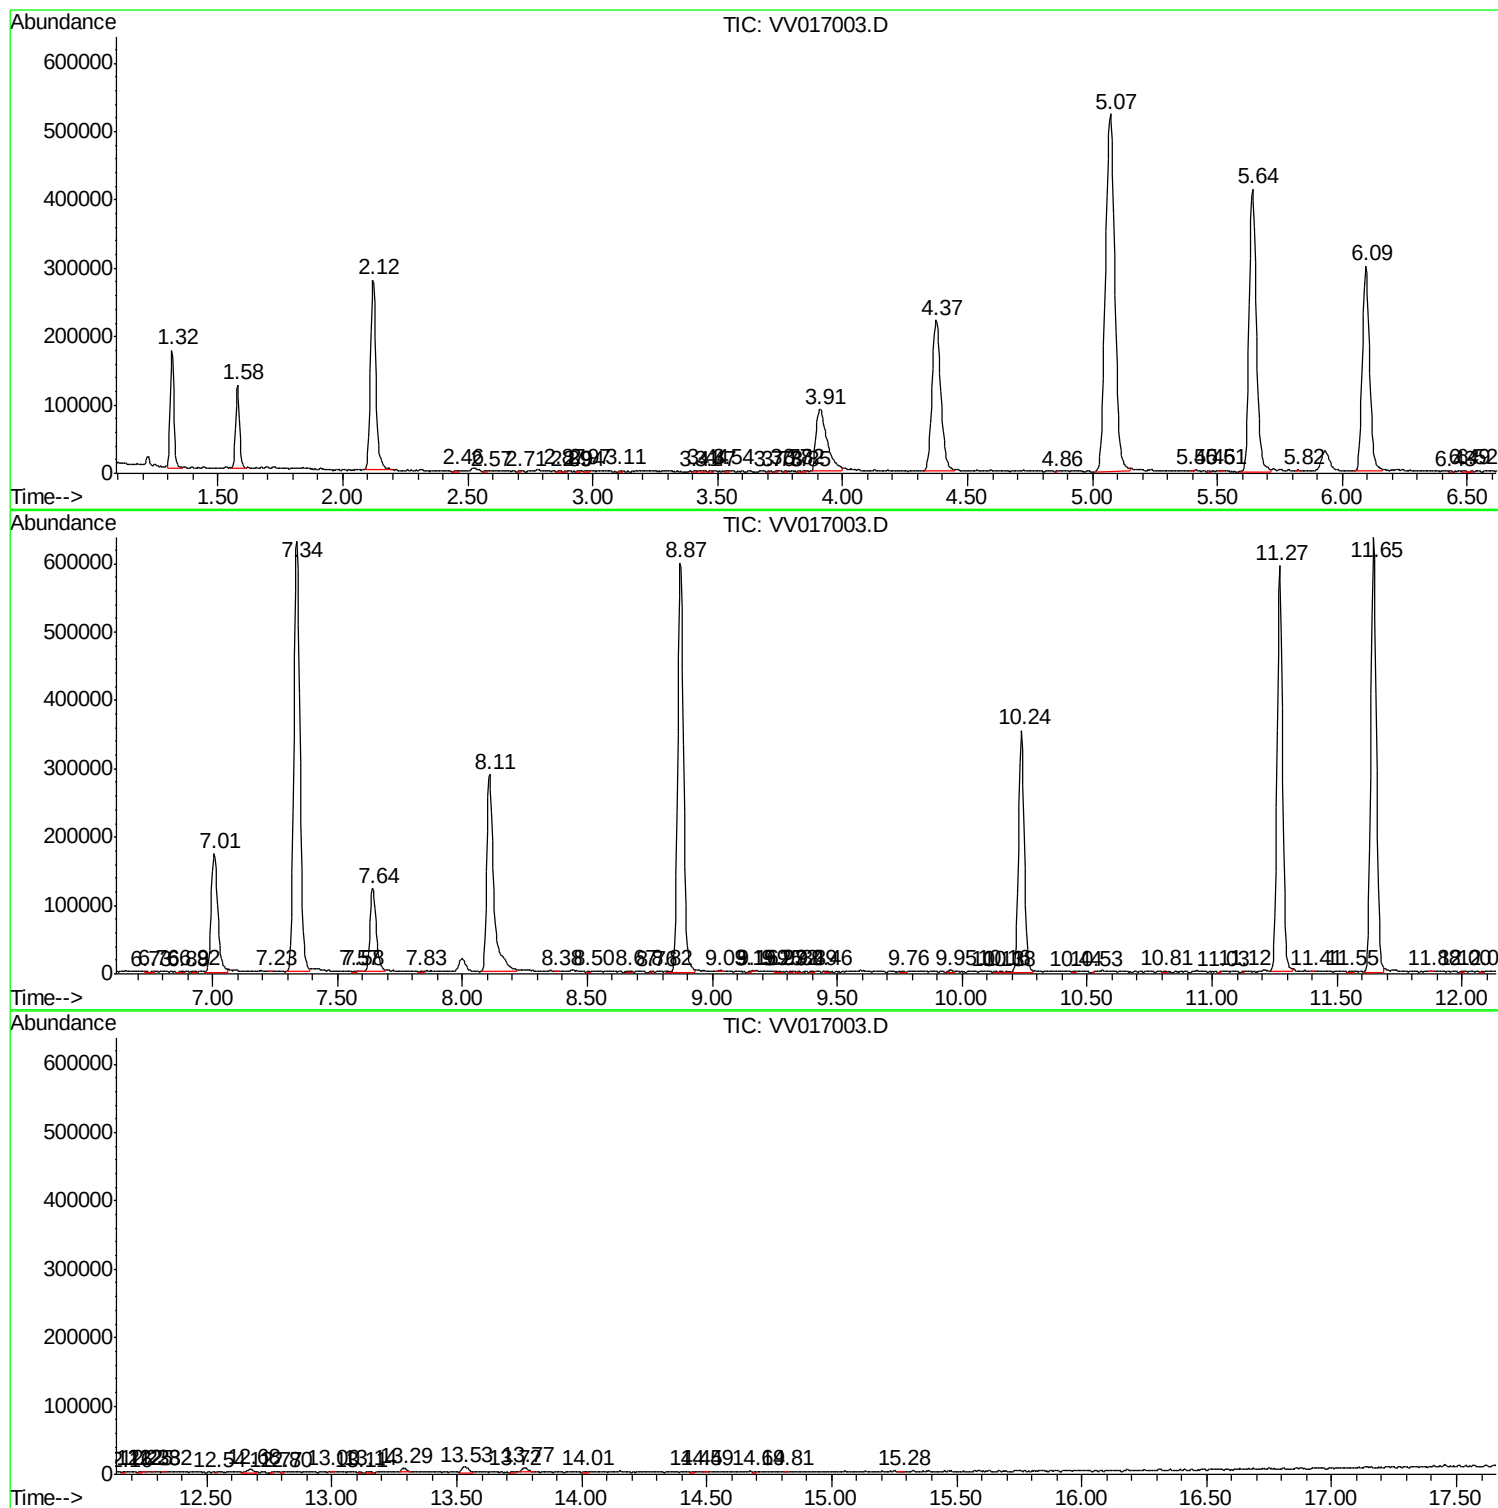

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061920\
Data File : VV017003.D
Acq On : 19 Jun 2020 16:39
Operator : SY/MD
Sample : VIBLK60
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK60

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061920\
Data File : VV017003.D
Acq On : 19 Jun 2020 16:39
Operator : SY/MD
Sample : VIBLK60
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK60

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc