

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017004.D
 Acq On : 19 Jun 2020 17:02
 Operator : SY/MD
 Sample : L3074-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	181755	176223	12.90%	1.574%
2	1.579	145	152	164	rVB	119595	132045	9.67%	1.179%
3	2.122	311	321	341	rBV	284921	433225	31.71%	3.869%
4	2.682	493	495	498	rBV3	1296	815	0.06%	0.007%
5	2.762	518	520	523	rBV3	1137	620	0.05%	0.006%
6	2.862	549	551	554	rVB4	972	478	0.03%	0.004%
7	2.958	579	581	583	rVV2	1188	584	0.04%	0.005%
8	3.010	595	597	599	rBV2	933	504	0.04%	0.005%
9	3.277	678	680	682	rBV3	973	499	0.04%	0.004%
10	3.309	686	690	691	rBV3	834	551	0.04%	0.005%
11	3.592	774	778	780	rBV4	1674	1330	0.10%	0.012%
12	3.637	789	792	793	rBV3	1176	530	0.04%	0.005%
13	3.688	806	808	811	rBV4	781	495	0.04%	0.004%
14	3.843	854	856	859	rBV4	724	416	0.03%	0.004%
15	3.907	864	876	903	rBV	93462	280673	20.54%	2.507%
16	4.241	977	980	982	rBV4	1354	1074	0.08%	0.010%
17	4.273	988	990	993	rBV3	1614	886	0.06%	0.008%
18	4.322	1003	1005	1006	rBV2	1264	454	0.03%	0.004%
19	4.376	1007	1022	1048	rVB	226566	557562	40.81%	4.979%
20	4.576	1081	1084	1085	rBV2	1144	727	0.05%	0.006%
21	4.942	1197	1198	1200	rBV2	858	376	0.03%	0.003%
22	4.990	1210	1213	1219	rBV6	1443	1852	0.14%	0.017%
23	5.016	1219	1221	1222	rBV2	1359	656	0.05%	0.006%
24	5.071	1222	1238	1265	rVV2	526839	1366187	100.00%	12.201%
25	5.592	1398	1400	1402	rBV2	926	479	0.04%	0.004%
26	5.643	1403	1416	1450	rVV	404837	818071	59.88%	7.306%
27	5.936	1495	1507	1522	rBV7	39051	89181	6.53%	0.796%
28	6.093	1543	1556	1580	rVV	306494	616749	45.14%	5.508%
29	6.395	1649	1650	1655	rVB3	1160	870	0.06%	0.008%
30	6.428	1655	1660	1661	rBV3	1366	1237	0.09%	0.011%
31	6.524	1687	1690	1698	rBV9	1896	1798	0.13%	0.016%
32	6.688	1739	1741	1744	rBV4	1298	775	0.06%	0.007%
33	6.717	1749	1750	1753	rVB3	1240	496	0.04%	0.004%
34	6.830	1783	1785	1787	rBV3	1071	450	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017004.D
 Acq On : 19 Jun 2020 17:02
 Operator : SY/MD
 Sample : L3074-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.961	1824	1826	1828	rBV3	907	405	0.03%	0.004%
36	7.006	1828	1840	1857	rBV	175400	318203	23.29%	2.842%
37	7.338	1931	1943	1959	rBV	645491	1091855	79.92%	9.751%
38	7.518	1997	1999	2000	rBV2	1215	503	0.04%	0.004%
39	7.547	2005	2008	2010	rBV3	1682	1085	0.08%	0.010%
40	7.643	2023	2038	2051	rBV	124635	217199	15.90%	1.940%
41	7.948	2130	2133	2134	rBV3	1804	1024	0.07%	0.009%
42	7.997	2137	2148	2164	rVB	600839	1009068	73.86%	9.012%
43	8.109	2173	2183	2218	rBV	289614	567380	41.53%	5.067%
44	8.601	2333	2336	2340	rVV5	1719	1272	0.09%	0.011%
45	8.620	2340	2342	2347	rVB4	1683	1187	0.09%	0.011%
46	8.656	2351	2353	2355	rBV3	1197	683	0.05%	0.006%
47	8.691	2362	2364	2368	rVB4	1607	1049	0.08%	0.009%
48	8.710	2368	2370	2375	rBV4	1109	680	0.05%	0.006%
49	8.820	2399	2404	2406	rBV4	1207	1064	0.08%	0.010%
50	8.871	2408	2420	2440	rBV	597855	977505	71.55%	8.730%
51	9.035	2469	2471	2474	rBV4	2097	1127	0.08%	0.010%
52	9.119	2494	2497	2498	rBV3	1131	672	0.05%	0.006%
53	9.415	2587	2589	2592	rBV3	756	431	0.03%	0.004%
54	9.485	2609	2611	2616	rBV4	1658	1271	0.09%	0.011%
55	9.508	2616	2618	2620	rVV3	1238	571	0.04%	0.005%
56	9.566	2631	2636	2639	rBV6	2142	2536	0.19%	0.023%
57	9.637	2656	2658	2661	rVB3	1433	464	0.03%	0.004%
58	9.685	2671	2673	2675	rBV3	1199	612	0.04%	0.005%
59	9.823	2713	2716	2718	rBV3	1566	916	0.07%	0.008%
60	9.852	2722	2725	2728	rVV5	1083	696	0.05%	0.006%
61	9.955	2750	2757	2759	rBV8	2731	3141	0.23%	0.028%
62	10.022	2774	2778	2779	rBV5	1610	1078	0.08%	0.010%
63	10.071	2791	2793	2794	rBV2	1347	410	0.03%	0.004%
64	10.238	2834	2845	2861	rBV	367510	569805	41.71%	5.089%
65	10.354	2878	2881	2882	rBV3	1151	595	0.04%	0.005%
66	10.444	2906	2909	2912	rBV4	1093	605	0.04%	0.005%
67	10.604	2953	2959	2962	rBV6	1826	2203	0.16%	0.020%
68	10.720	2992	2995	2998	rBV3	1102	1182	0.09%	0.011%
69	10.762	3005	3008	3010	rBV4	1333	891	0.07%	0.008%
70	10.788	3013	3016	3019	rBV3	1473	681	0.05%	0.006%
71	10.852	3032	3036	3040	rBV7	1693	1815	0.13%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017004.D
 Acq On : 19 Jun 2020 17:02
 Operator : SY/MD
 Sample : L3074-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.919	3053	3057	3058	rBV3	1017	561	0.04%	0.005%
73	11.029	3088	3091	3094	rBV5	1166	1085	0.08%	0.010%
74	11.270	3155	3166	3188	rBV	573958	892027	65.29%	7.966%
75	11.646	3270	3283	3299	rBV	644004	1006371	73.66%	8.988%
76	11.839	3341	3343	3345	rBV3	1371	859	0.06%	0.008%
77	11.971	3382	3384	3389	rVB5	995	677	0.05%	0.006%
78	12.013	3392	3397	3398	rBV5	1155	1034	0.08%	0.009%
79	12.032	3401	3403	3405	rBV2	1188	649	0.05%	0.006%
80	12.234	3465	3466	3469	rBV2	880	535	0.04%	0.005%
81	12.267	3473	3476	3480	rBV4	2114	1541	0.11%	0.014%
82	12.382	3509	3512	3516	rVB4	1488	1056	0.08%	0.009%
83	12.405	3516	3519	3520	rBV2	1160	625	0.05%	0.006%
84	12.424	3523	3525	3527	rBV3	716	415	0.03%	0.004%
85	12.505	3548	3550	3557	rVB6	2866	1834	0.13%	0.016%
86	12.543	3560	3562	3567	rVB3	1287	762	0.06%	0.007%
87	12.807	3640	3644	3646	rBV4	1934	1289	0.09%	0.012%
88	12.884	3666	3668	3672	rBV4	1047	814	0.06%	0.007%
89	12.919	3676	3679	3681	rBV4	1416	787	0.06%	0.007%
90	12.955	3689	3690	3692	rBV2	1132	393	0.03%	0.004%
91	13.003	3703	3705	3709	rVB4	1564	955	0.07%	0.009%
92	13.022	3709	3711	3714	rBV3	737	476	0.03%	0.004%
93	13.260	3783	3785	3787	rBV2	1137	659	0.05%	0.006%
94	13.395	3824	3827	3831	rBV4	1434	1547	0.11%	0.014%
95	13.623	3896	3898	3899	rBV2	1135	377	0.03%	0.003%
96	13.730	3928	3931	3932	rBV3	1316	693	0.05%	0.006%
97	13.768	3938	3943	3952	rBV3	3204	5482	0.40%	0.049%
98	13.916	3987	3989	3993	rVB4	2677	1396	0.10%	0.012%
99	14.360	4125	4127	4128	rBV2	1160	393	0.03%	0.004%
100	14.730	4239	4242	4246	rBV6	1938	1280	0.09%	0.011%


Sum of corrected areas: 11197304

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061920\
Data File : VV017004.D
Acq On : 19 Jun 2020 17:02
Operator : SY/MD
Sample : L3074-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9M06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

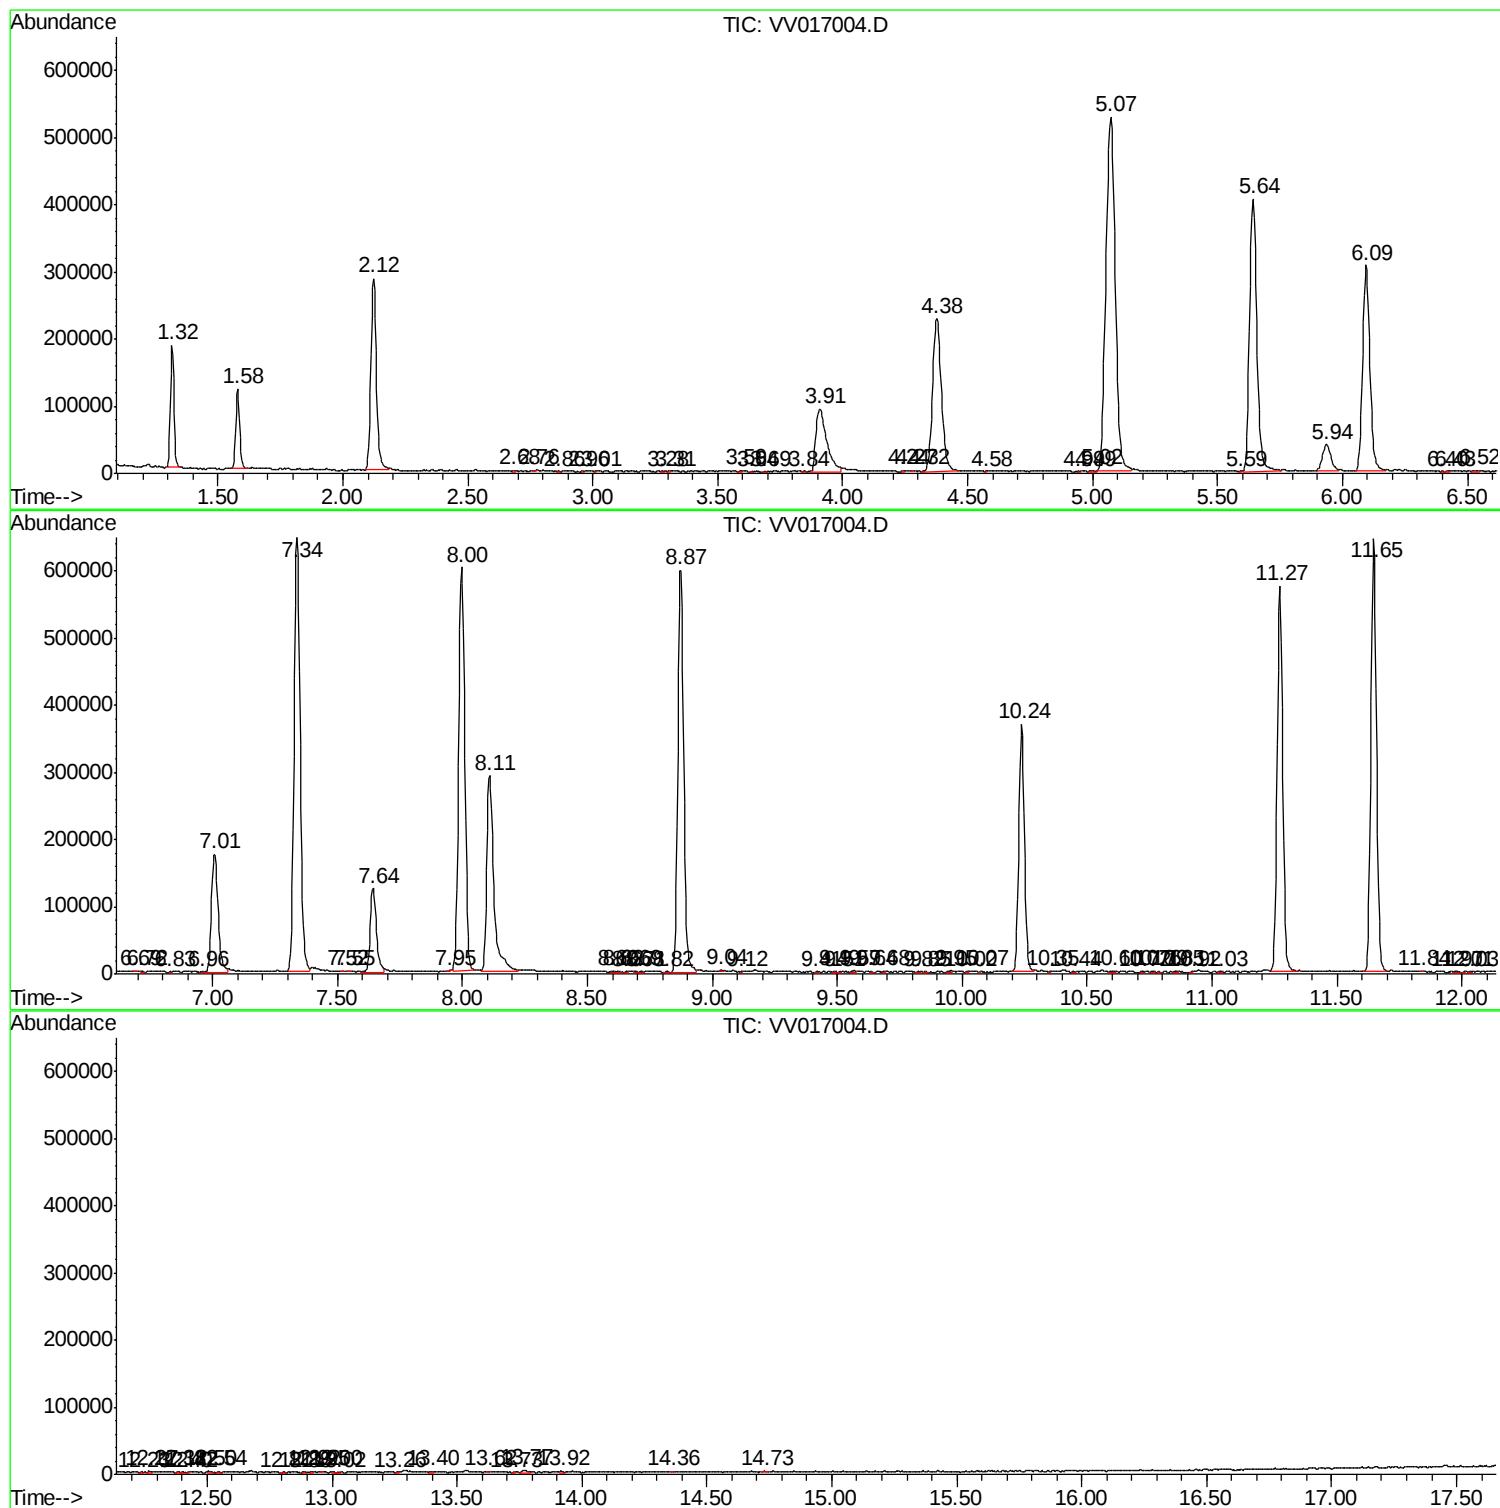

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017004.D
Acq On : 19 Jun 2020 17:02
Operator : SY/MD
Sample : L3074-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017004.D
Acq On : 19 Jun 2020 17:02
Operator : SY/MD
Sample : L3074-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc