

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017005.D
 Acq On : 19 Jun 2020 17:25
 Operator : SY/MD
 Sample : L3074-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	82	rVB	173839	180999	13.45%	1.610%
2	1.579	145	152	164	rVB	122264	135467	10.07%	1.205%
3	2.123	312	321	338	rBV	284864	422648	31.41%	3.760%
4	2.280	367	370	373	rBV4	1957	1325	0.10%	0.012%
5	2.756	516	518	521	rVB4	1229	722	0.05%	0.006%
6	2.885	555	558	561	rBV5	923	855	0.06%	0.008%
7	2.971	582	585	590	rBV7	958	955	0.07%	0.008%
8	3.036	602	605	610	rBV6	1128	1163	0.09%	0.010%
9	3.058	610	612	616	rVB3	1080	692	0.05%	0.006%
10	3.081	616	619	621	rBV4	1024	668	0.05%	0.006%
11	3.119	628	631	634	rVB4	1274	860	0.06%	0.008%
12	3.142	634	638	639	rBV4	1214	917	0.07%	0.008%
13	3.212	656	660	661	rBV4	1422	885	0.07%	0.008%
14	3.499	747	749	755	rVB6	1319	802	0.06%	0.007%
15	3.585	774	776	778	rBV3	1356	674	0.05%	0.006%
16	3.788	834	839	840	rBV5	1225	826	0.06%	0.007%
17	3.910	865	877	904	rBV2	94675	283929	21.10%	2.526%
18	4.264	985	987	989	rBV3	1349	691	0.05%	0.006%
19	4.376	1004	1022	1044	rBV2	224966	552653	41.08%	4.916%
20	4.515	1063	1065	1071	rBV7	1600	846	0.06%	0.008%
21	4.608	1092	1094	1099	rBV6	912	726	0.05%	0.006%
22	4.659	1106	1110	1111	rBV4	1826	1208	0.09%	0.011%
23	4.740	1132	1135	1138	rBV4	1911	1145	0.09%	0.010%
24	4.785	1146	1149	1153	rBV6	1637	1321	0.10%	0.012%
25	5.074	1222	1239	1262	rBV2	519355	1345375	100.00%	11.968%
26	5.547	1383	1386	1388	rVB4	1530	781	0.06%	0.007%
27	5.640	1401	1415	1437	rBV	397726	802682	59.66%	7.140%
28	5.936	1493	1507	1521	rBV5	37189	91150	6.78%	0.811%
29	6.093	1543	1556	1575	rBV	305147	607360	45.14%	5.403%
30	6.431	1658	1661	1664	rBV4	1504	971	0.07%	0.009%
31	6.614	1715	1718	1722	rBV5	1559	1521	0.11%	0.014%
32	6.756	1760	1762	1765	rVB4	1600	771	0.06%	0.007%
33	6.781	1765	1770	1771	rBV3	1185	777	0.06%	0.007%
34	6.814	1776	1780	1784	rBV7	1366	971	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017005.D
 Acq On : 19 Jun 2020 17:25
 Operator : SY/MD
 Sample : L3074-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.007	1829	1840	1861	rBV	173303	311420	23.15%	2.770%
36	7.164	1885	1889	1891	rBV4	1443	1213	0.09%	0.011%
37	7.338	1930	1943	1965	rBV	631562	1090458	81.05%	9.700%
38	7.643	2028	2038	2055	rBV2	119344	207313	15.41%	1.844%
39	7.997	2135	2148	2163	rVV	669771	1112724	82.71%	9.898%
40	8.109	2173	2183	2211	rBV	296150	564942	41.99%	5.025%
41	8.415	2275	2278	2280	rBV4	1500	874	0.06%	0.008%
42	8.470	2291	2295	2297	rBV5	1534	1198	0.09%	0.011%
43	8.701	2362	2367	2371	rBV7	2144	1866	0.14%	0.017%
44	8.794	2393	2396	2398	rBV3	1229	749	0.06%	0.007%
45	8.871	2410	2420	2443	rBV	590113	960653	71.40%	8.546%
46	9.158	2505	2509	2510	rBV4	1593	1096	0.08%	0.010%
47	9.187	2516	2518	2523	rBV5	1623	1035	0.08%	0.009%
48	9.309	2553	2556	2560	rBV3	1111	924	0.07%	0.008%
49	9.334	2560	2564	2566	rBV4	989	751	0.06%	0.007%
50	9.363	2570	2573	2574	rBV2	1491	893	0.07%	0.008%
51	9.418	2585	2590	2591	rBV4	1147	904	0.07%	0.008%
52	9.601	2644	2647	2650	rBV5	1485	945	0.07%	0.008%
53	9.653	2657	2663	2665	rBV5	1813	1439	0.11%	0.013%
54	9.810	2708	2712	2715	rVB6	1212	842	0.06%	0.007%
55	10.019	2772	2777	2778	rBV4	1456	1083	0.08%	0.010%
56	10.158	2816	2820	2822	rBV4	1442	937	0.07%	0.008%
57	10.174	2822	2825	2827	rVV4	1447	854	0.06%	0.008%
58	10.238	2833	2845	2863	rBV	366291	574377	42.69%	5.109%
59	10.395	2890	2894	2897	rBV5	2650	2551	0.19%	0.023%
60	10.469	2913	2917	2919	rBV3	1644	1137	0.08%	0.010%
61	10.556	2942	2944	2949	rVV4	1606	1308	0.10%	0.012%
62	10.585	2951	2953	2955	rBV3	1471	782	0.06%	0.007%
63	10.640	2966	2970	2974	rBV6	1425	1354	0.10%	0.012%
64	10.836	3028	3031	3035	rBV6	1115	1135	0.08%	0.010%
65	10.875	3039	3043	3046	rBV5	1685	1357	0.10%	0.012%
66	10.903	3050	3052	3055	rBV4	1175	746	0.06%	0.007%
67	10.929	3059	3060	3063	rVB2	1706	867	0.06%	0.008%
68	10.945	3063	3065	3070	rBV6	1793	1154	0.09%	0.010%
69	11.022	3086	3089	3095	rBV4	1182	1168	0.09%	0.010%
70	11.199	3142	3144	3149	rBV4	1915	1940	0.14%	0.017%
71	11.270	3154	3166	3188	rBV	582609	901013	66.97%	8.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017005.D
 Acq On : 19 Jun 2020 17:25
 Operator : SY/MD
 Sample : L3074-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.540	3247	3250	3253	rBV4	1803	1590	0.12%	0.014%
73	11.646	3272	3283	3302	rVB	650746	1009497	75.03%	8.980%
74	11.807	3331	3333	3336	rBV4	1290	848	0.06%	0.008%
75	11.878	3353	3355	3360	rVB4	1516	1080	0.08%	0.010%
76	11.974	3383	3385	3389	rVB4	1385	747	0.06%	0.007%
77	12.051	3407	3409	3411	rBV3	1203	669	0.05%	0.006%
78	12.100	3418	3424	3431	rVB9	1820	2978	0.22%	0.026%
79	12.302	3484	3487	3491	rBV5	1413	1457	0.11%	0.013%
80	12.347	3498	3501	3502	rBV3	1352	658	0.05%	0.006%
81	12.450	3529	3533	3536	rBV5	1227	1122	0.08%	0.010%
82	12.505	3548	3550	3554	rVB4	1945	1066	0.08%	0.009%
83	12.572	3569	3571	3575	rVB4	1683	879	0.07%	0.008%
84	12.598	3575	3579	3581	rBV4	942	752	0.06%	0.007%
85	12.682	3602	3605	3607	rBV3	1162	775	0.06%	0.007%
86	12.759	3624	3629	3630	rBV3	1119	865	0.06%	0.008%
87	13.000	3702	3704	3707	rBV4	1231	749	0.06%	0.007%
88	13.135	3742	3746	3747	rBV3	1432	908	0.07%	0.008%
89	13.280	3787	3791	3795	rBV7	2568	2761	0.21%	0.025%
90	13.498	3857	3859	3861	rBV2	1655	976	0.07%	0.009%
91	13.714	3922	3926	3927	rBV3	1223	850	0.06%	0.008%
92	13.768	3939	3943	3944	rBV3	1725	1224	0.09%	0.011%
93	13.858	3968	3971	3973	rBV5	1240	846	0.06%	0.008%
94	13.968	4001	4005	4009	rVB7	1192	1013	0.08%	0.009%
95	14.003	4014	4016	4018	rBV2	1214	719	0.05%	0.006%
96	14.312	4108	4112	4115	rBV6	1791	1231	0.09%	0.011%
97	14.363	4124	4128	4131	rBV5	1391	923	0.07%	0.008%
98	14.444	4149	4153	4155	rBV4	1196	893	0.07%	0.008%
99	14.736	4241	4244	4246	rBV3	1601	1095	0.08%	0.010%
100	14.981	4318	4320	4323	rBV3	1551	1009	0.07%	0.009%


Sum of corrected areas: 11241518

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061920\
Data File : VV017005.D
Acq On : 19 Jun 2020 17:25
Operator : SY/MD
Sample : L3074-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

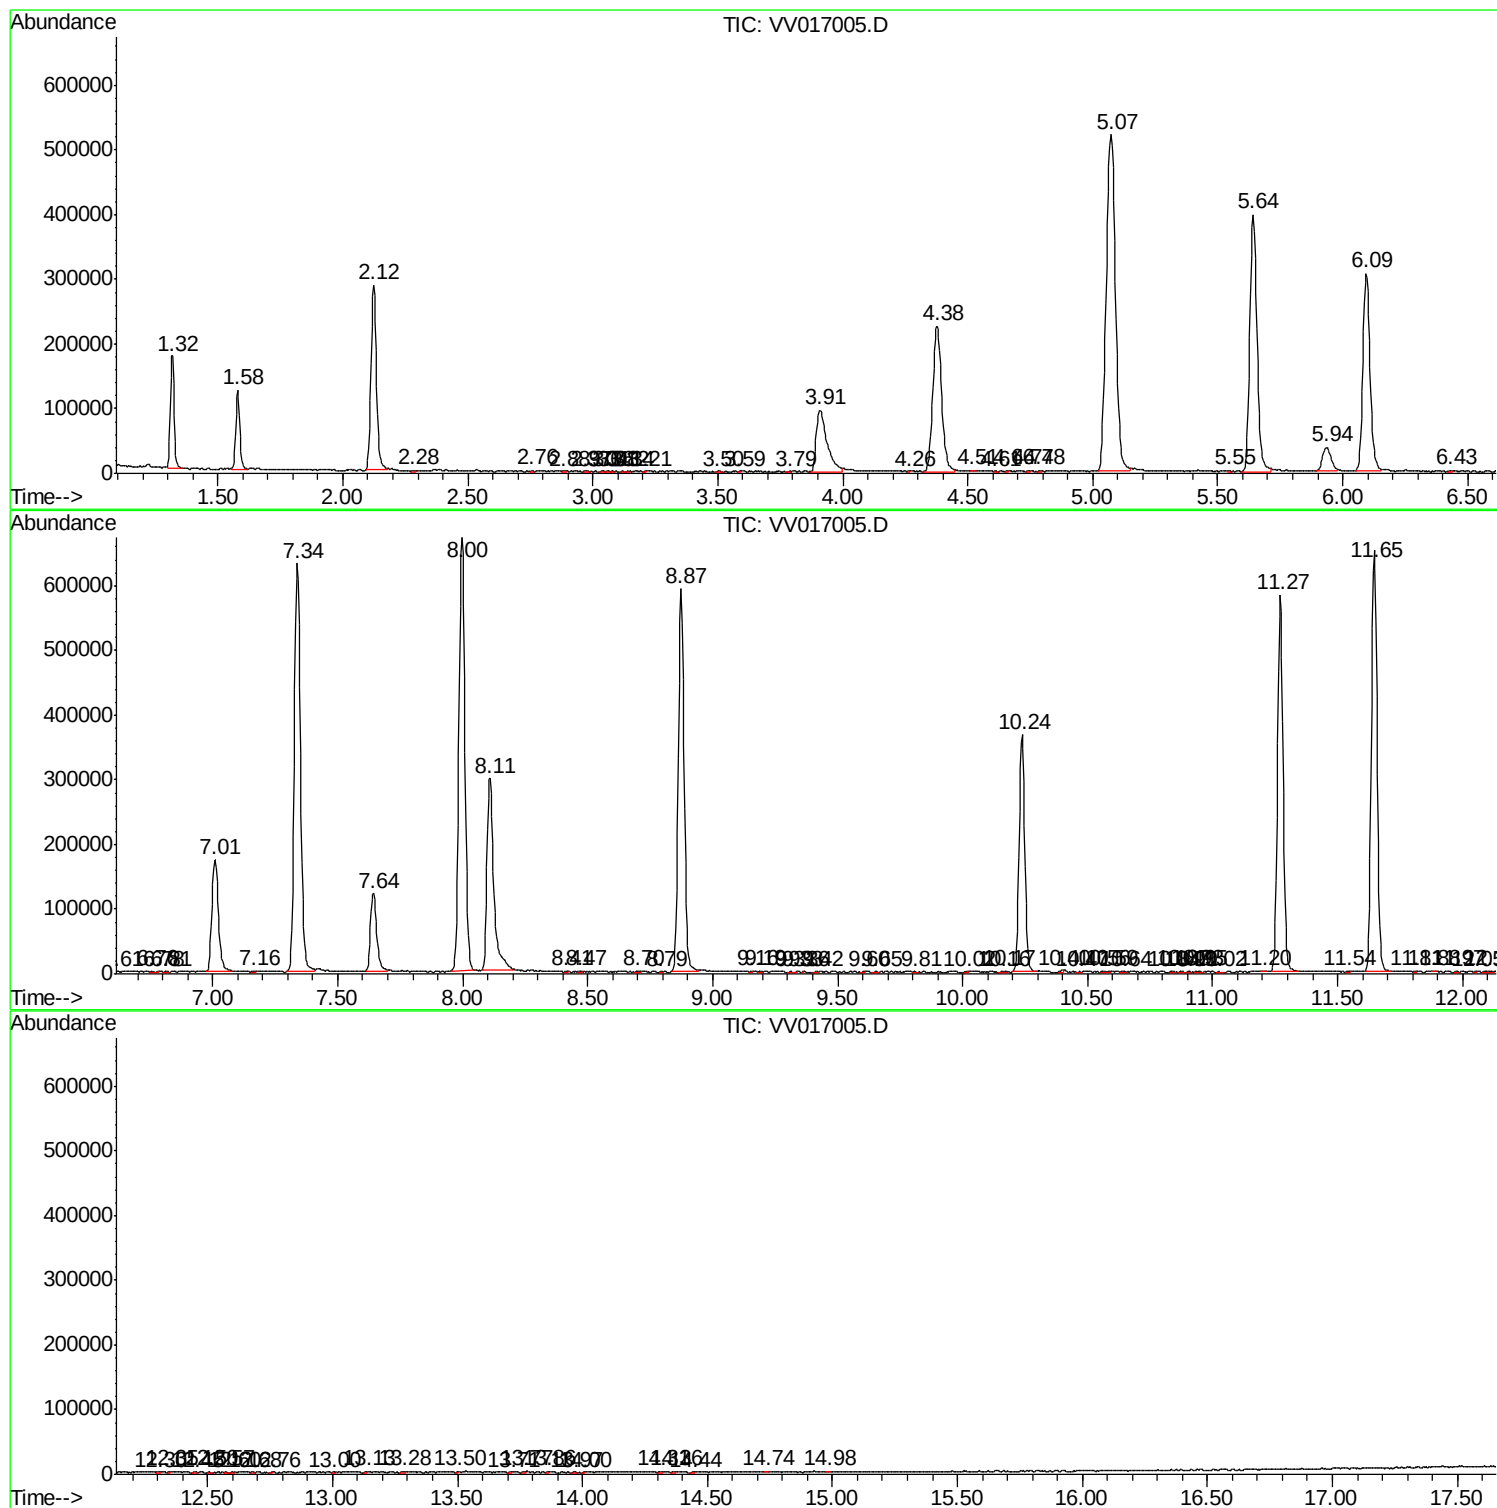

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017005.D
Acq On : 19 Jun 2020 17:25
Operator : SY/MD
Sample : L3074-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M09

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017005.D
Acq On : 19 Jun 2020 17:25
Operator : SY/MD
Sample : L3074-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M09

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc