

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017008.D
 Acq On : 19 Jun 2020 18:35
 Operator : SY/MD
 Sample : L3074-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	174287	178461	12.68%	1.538%
2	1.579	145	152	163	rVB	116583	125836	8.94%	1.084%
3	2.122	311	321	340	rBV	286301	429486	30.53%	3.701%
4	2.527	440	447	450	rBV7	1840	2435	0.17%	0.021%
5	2.878	551	556	559	rVB6	1225	1131	0.08%	0.010%
6	2.894	559	561	564	rBV5	1714	1282	0.09%	0.011%
7	3.019	596	600	606	rVB8	1305	1393	0.10%	0.012%
8	3.113	625	629	632	rBV5	1619	1345	0.10%	0.012%
9	3.132	632	635	638	rVB5	856	614	0.04%	0.005%
10	3.196	652	655	657	rVV4	1773	1025	0.07%	0.009%
11	3.222	661	663	666	rVB3	1410	897	0.06%	0.008%
12	3.296	680	686	688	rVV6	1022	967	0.07%	0.008%
13	3.322	691	694	699	rVV6	1269	1072	0.08%	0.009%
14	3.460	733	737	741	rBV7	1049	840	0.06%	0.007%
15	3.508	747	752	754	rBV5	1623	1329	0.09%	0.011%
16	3.527	754	758	761	rVB3	1113	867	0.06%	0.007%
17	3.682	803	806	809	rBV3	824	761	0.05%	0.007%
18	3.724	815	819	823	rBV6	1194	1075	0.08%	0.009%
19	3.746	823	826	828	rBV3	1428	720	0.05%	0.006%
20	3.910	866	877	904	rBV2	92937	295987	21.04%	2.551%
21	4.376	1007	1022	1048	rVV	225255	547954	38.95%	4.722%
22	4.576	1082	1084	1086	rBV3	1305	695	0.05%	0.006%
23	4.724	1126	1130	1133	rVB5	1332	989	0.07%	0.009%
24	4.875	1173	1177	1180	rBV5	2009	1673	0.12%	0.014%
25	4.910	1186	1188	1191	rVB3	1205	836	0.06%	0.007%
26	4.933	1191	1195	1197	rBV5	1495	1180	0.08%	0.010%
27	4.971	1203	1207	1211	rBV6	1346	1229	0.09%	0.011%
28	5.071	1221	1238	1263	rBV2	525340	1365947	97.09%	11.770%
29	5.511	1370	1375	1377	rBV6	979	837	0.06%	0.007%
30	5.559	1384	1390	1392	rBV6	1592	1708	0.12%	0.015%
31	5.640	1403	1415	1436	rBV	400583	790565	56.19%	6.812%
32	5.936	1492	1507	1524	rVV5	55303	130213	9.26%	1.122%
33	6.093	1541	1556	1583	rBV	304172	621793	44.19%	5.358%
34	6.402	1647	1652	1655	rBV7	2275	2029	0.14%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017008.D
 Acq On : 19 Jun 2020 18:35
 Operator : SY/MD
 Sample : L3074-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.473	1671	1674	1678	rBV5	1525	1092	0.08%	0.009%
36	6.617	1713	1719	1722	rVB7	1285	1174	0.08%	0.010%
37	6.653	1728	1730	1735	rBV4	1395	936	0.07%	0.008%
38	6.768	1763	1766	1769	rBV3	1643	1239	0.09%	0.011%
39	7.006	1826	1840	1861	rBV	172876	314083	22.32%	2.706%
40	7.180	1889	1894	1897	rBV6	2138	1731	0.12%	0.015%
41	7.196	1897	1899	1902	rBV2	1676	972	0.07%	0.008%
42	7.296	1926	1930	1931	rBV4	1263	726	0.05%	0.006%
43	7.338	1931	1943	1961	rBV	633891	1094882	77.82%	9.435%
44	7.643	2026	2038	2055	rBV	124001	215359	15.31%	1.856%
45	7.820	2091	2093	2095	rBV3	1377	686	0.05%	0.006%
46	7.839	2097	2099	2102	rVB5	1638	733	0.05%	0.006%
47	7.997	2129	2148	2164	rBV	842679	1406932	100.00%	12.124%
48	8.109	2173	2183	2214	rBV2	300145	564868	40.15%	4.867%
49	8.392	2269	2271	2273	rBV3	1118	654	0.05%	0.006%
50	8.479	2295	2298	2301	rVB3	1361	973	0.07%	0.008%
51	8.511	2302	2308	2310	rBV5	1699	1600	0.11%	0.014%
52	8.588	2330	2332	2335	rVB4	1357	848	0.06%	0.007%
53	8.665	2354	2356	2359	rBB4	1463	727	0.05%	0.006%
54	8.871	2409	2420	2438	rBV	597018	955647	67.92%	8.235%
55	9.167	2509	2512	2514	rBV3	1818	1067	0.08%	0.009%
56	9.591	2643	2644	2652	rVB7	1842	1177	0.08%	0.010%
57	9.665	2664	2667	2670	rBV5	1057	787	0.06%	0.007%
58	9.701	2675	2678	2680	rVV5	1513	874	0.06%	0.008%
59	9.923	2743	2747	2749	rBV5	1402	1070	0.08%	0.009%
60	9.948	2752	2755	2757	rBV5	871	678	0.05%	0.006%
61	10.238	2833	2845	2863	rBV	364662	572182	40.67%	4.930%
62	10.784	3013	3015	3017	rBV3	1343	785	0.06%	0.007%
63	10.826	3025	3028	3033	rVB5	962	952	0.07%	0.008%
64	10.852	3033	3036	3040	rBV4	2115	1609	0.11%	0.014%
65	10.900	3048	3051	3053	rBV2	1141	758	0.05%	0.007%
66	10.935	3059	3062	3065	rBV4	1782	1500	0.11%	0.013%
67	11.090	3107	3110	3112	rBV4	1238	939	0.07%	0.008%
68	11.161	3130	3132	3135	rVB3	1429	588	0.04%	0.005%
69	11.270	3153	3166	3185	rBV	582993	887633	63.09%	7.649%
70	11.453	3218	3223	3224	rBV3	933	863	0.06%	0.007%
71	11.556	3253	3255	3257	rBV3	1068	764	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017008.D
 Acq On : 19 Jun 2020 18:35
 Operator : SY/MD
 Sample : L3074-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M14

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3300	rBV	649613	1021924	72.63%	8.806%
73	11.833	3339	3341	3344	rVB4	2190	1031	0.07%	0.009%
74	11.855	3344	3348	3351	rBV4	1318	1060	0.08%	0.009%
75	12.000	3390	3393	3395	rBV4	1143	646	0.05%	0.006%
76	12.196	3451	3454	3458	rVB6	986	699	0.05%	0.006%
77	12.212	3458	3459	3463	rVB3	1178	647	0.05%	0.006%
78	12.231	3463	3465	3466	rBV2	1246	628	0.04%	0.005%
79	12.450	3529	3533	3535	rBV4	1568	1241	0.09%	0.011%
80	12.482	3539	3543	3547	rBV5	1377	1270	0.09%	0.011%
81	12.562	3566	3568	3570	rVB3	1419	664	0.05%	0.006%
82	12.588	3573	3576	3577	rBV3	1248	741	0.05%	0.006%
83	12.759	3625	3629	3630	rBV3	1044	708	0.05%	0.006%
84	12.804	3638	3643	3646	rVB7	1569	1128	0.08%	0.010%
85	12.826	3646	3650	3652	rBV3	1409	1014	0.07%	0.009%
86	12.878	3664	3666	3669	rBV3	1534	907	0.06%	0.008%
87	13.222	3771	3773	3775	rBV4	1219	603	0.04%	0.005%
88	13.296	3793	3796	3798	rBV4	1392	887	0.06%	0.008%
89	13.443	3838	3842	3845	rBV5	1252	1117	0.08%	0.010%
90	13.537	3867	3871	3872	rBV3	1306	906	0.06%	0.008%
91	13.749	3934	3937	3938	rBV3	1322	932	0.07%	0.008%
92	13.932	3991	3994	3997	rBV4	1011	728	0.05%	0.006%
93	14.013	4013	4019	4024	rBV7	1513	1819	0.13%	0.016%
94	14.292	4099	4106	4107	rBV6	1779	2011	0.14%	0.017%
95	14.514	4172	4175	4176	rBV3	1067	648	0.05%	0.006%
96	14.765	4251	4253	4256	rVB4	1687	715	0.05%	0.006%
97	15.035	4334	4337	4338	rBV4	1434	816	0.06%	0.007%
98	15.222	4390	4395	4399	rBV9	2230	2366	0.17%	0.020%
99	15.263	4404	4408	4409	rBV3	1452	939	0.07%	0.008%
100	15.466	4469	4471	4476	rBV6	1565	932	0.07%	0.008%


Sum of corrected areas: 11604986

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061920\
Data File : VV017008.D
Acq On : 19 Jun 2020 18:35
Operator : SY/MD
Sample : L3074-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M14

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

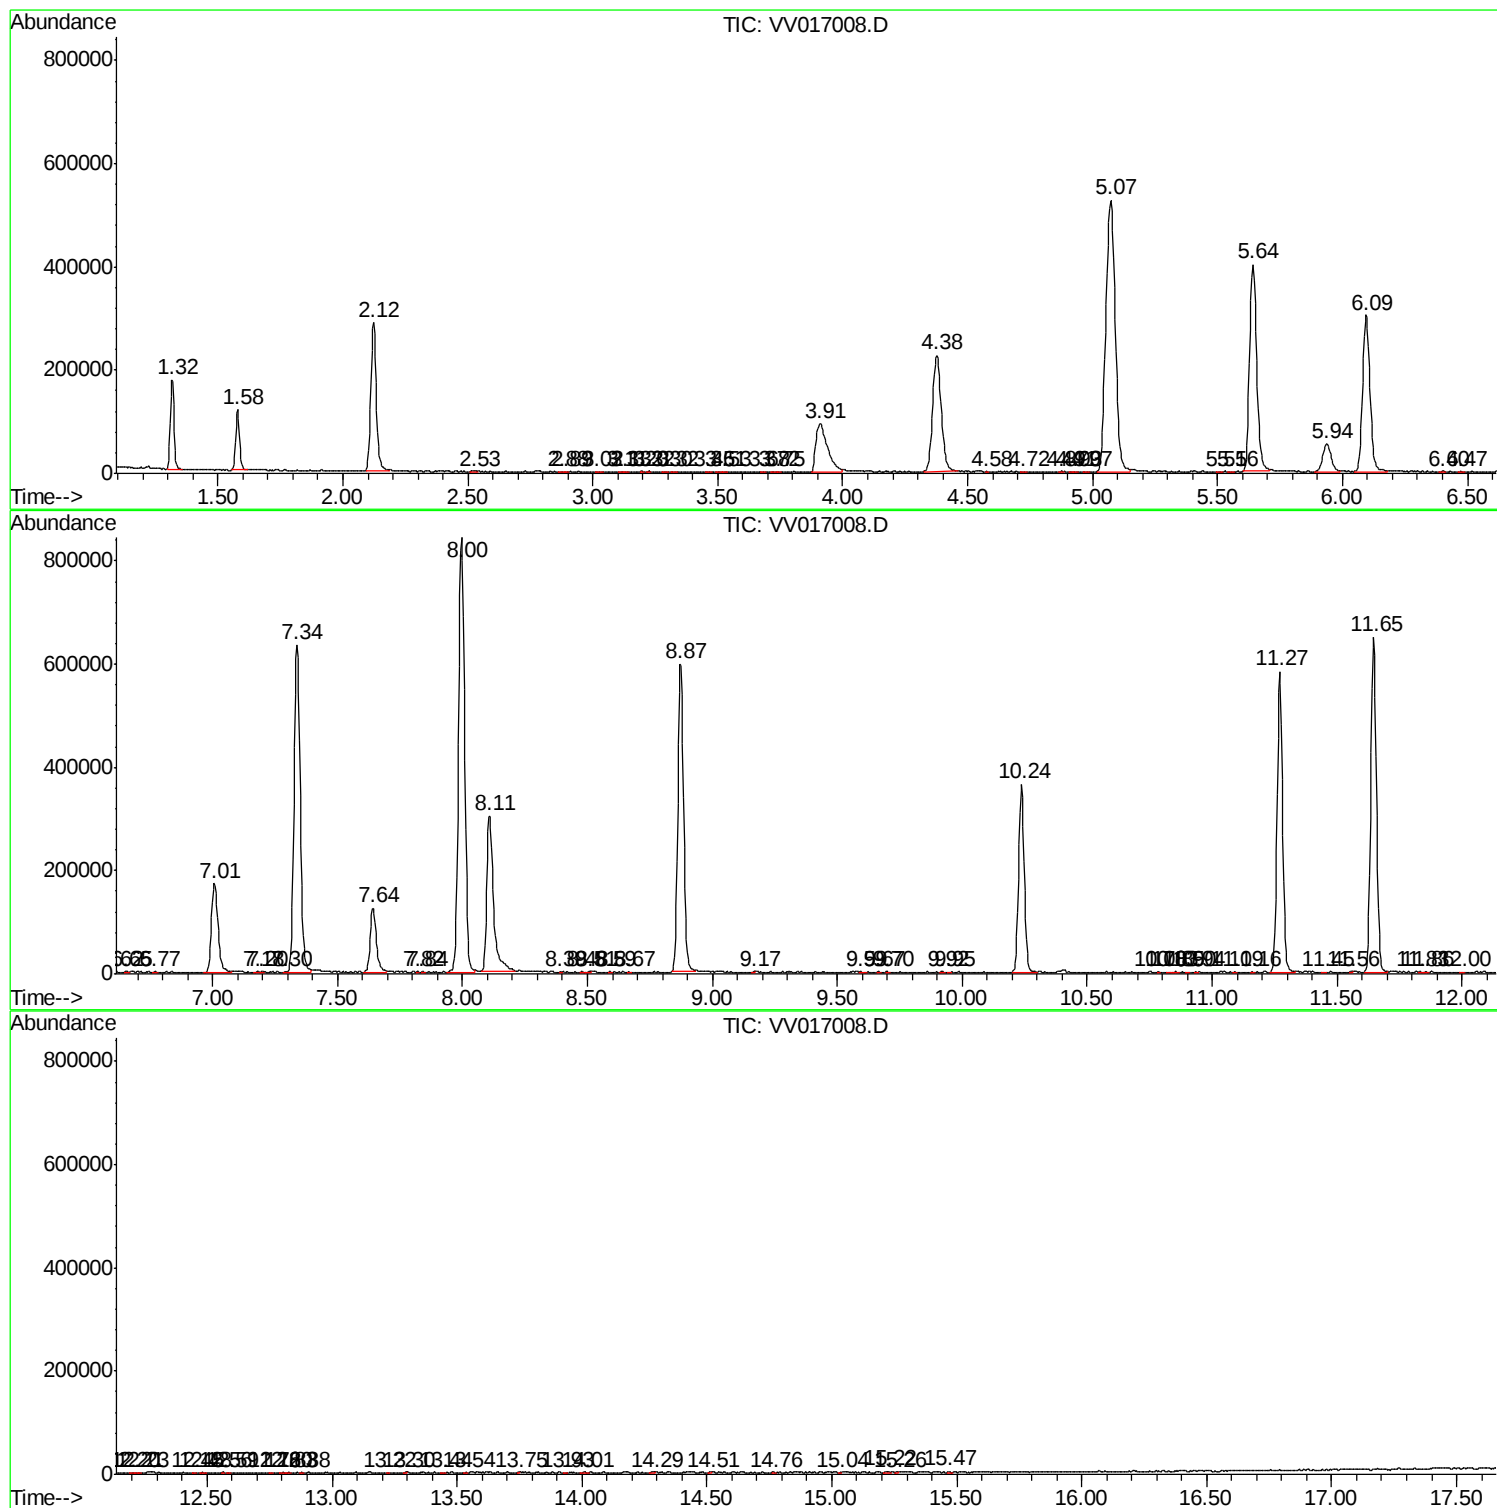

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017008.D
Acq On : 19 Jun 2020 18:35
Operator : SY/MD
Sample : L3074-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M14

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017008.D
Acq On : 19 Jun 2020 18:35
Operator : SY/MD
Sample : L3074-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M14

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc