

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017009.D
 Acq On : 19 Jun 2020 18:58
 Operator : SY/MD
 Sample : L3074-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	89	rVB	3221338	3318597	2.92%	1.292%
2	1.579	147	152	167	rVB	137190	159862	0.14%	0.062%
3	2.126	313	322	338	rVB3	356192	579767	0.51%	0.226%
4	2.782	515	526	545	rBV2	347204	623832	0.55%	0.243%
5	3.335	694	698	701	rBV5	1390	1054	0.00%	0.000%
6	3.380	708	712	716	rBV6	1259	1179	0.00%	0.000%
7	3.447	731	733	734	rBV2	955	403	0.00%	0.000%
8	3.492	745	747	749	rBV3	940	517	0.00%	0.000%
9	3.511	749	753	754	rVV4	881	631	0.00%	0.000%
10	3.550	762	765	770	rVB7	1010	908	0.00%	0.000%
11	3.585	774	776	777	rBV	1040	371	0.00%	0.000%
12	3.682	803	806	808	rBV3	1114	688	0.00%	0.000%
13	3.701	808	812	816	rBV5	1967	1164	0.00%	0.000%
14	3.720	816	818	820	rBV3	1438	804	0.00%	0.000%
15	3.775	833	835	838	rBV4	1270	691	0.00%	0.000%
16	3.791	838	840	844	rBV5	1175	902	0.00%	0.000%
17	3.827	849	851	852	rBV2	1062	469	0.00%	0.000%
18	3.942	865	887	941	rBV2	32243700	85160940	74.85%	33.147%
19	4.376	1011	1022	1046	rVB	244710	590420	0.52%	0.230%
20	5.000	1210	1216	1217	rBV6	1234	922	0.00%	0.000%
21	5.074	1221	1239	1272	rBV2	561527	1523548	1.34%	0.593%
22	5.428	1347	1349	1354	rVB6	1976	1534	0.00%	0.001%
23	5.482	1365	1366	1369	rBV3	880	579	0.00%	0.000%
24	5.643	1402	1416	1440	rBV	449167	899746	0.79%	0.350%
25	5.942	1491	1509	1543	rBV	21438457	42909005	37.72%	16.702%
26	6.097	1547	1557	1575	rVB	330503	666658	0.59%	0.259%
27	6.550	1694	1698	1699	rBV3	1410	1047	0.00%	0.000%
28	6.605	1713	1715	1716	rBV2	1725	476	0.00%	0.000%
29	6.711	1747	1748	1750	rBV2	1654	782	0.00%	0.000%
30	6.933	1814	1817	1818	rBV2	1124	439	0.00%	0.000%
31	7.006	1830	1840	1856	rBV	189277	334774	0.29%	0.130%
32	7.161	1885	1888	1889	rBV3	1460	806	0.00%	0.000%
33	7.338	1931	1943	1958	rBV	700756	1194503	1.05%	0.465%
34	7.643	2027	2038	2054	rBV	142034	240136	0.21%	0.093%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017009.D
 Acq On : 19 Jun 2020 18:58
 Operator : SY/MD
 Sample : L3074-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.913	2119	2122	2125	rBV5	1620	1195	0.00%	0.000%
36	7.939	2128	2130	2131	rBV2	1465	590	0.00%	0.000%
37	8.019	2131	2155	2174	rVV	55776262	113769284	100.00%	44.283%
38	8.106	2176	2182	2215	rVB	399626	735696	0.65%	0.286%
39	8.875	2409	2421	2444	rBV	706192	1155543	1.02%	0.450%
40	9.241	2533	2535	2536	rBV2	1143	453	0.00%	0.000%
41	9.405	2583	2586	2590	rVB6	1207	855	0.00%	0.000%
42	9.424	2590	2592	2593	rBV2	1364	678	0.00%	0.000%
43	9.672	2666	2669	2672	rBV4	1638	1509	0.00%	0.001%
44	9.730	2684	2687	2692	rBV6	1624	1418	0.00%	0.001%
45	9.794	2704	2707	2709	rBV5	1064	653	0.00%	0.000%
46	9.891	2735	2737	2739	rVB2	1631	704	0.00%	0.000%
47	9.903	2739	2741	2744	rBV3	1341	901	0.00%	0.000%
48	10.103	2798	2803	2804	rBV6	1700	1221	0.00%	0.000%
49	10.238	2831	2845	2857	rBV	430304	679122	0.60%	0.264%
50	10.588	2952	2954	2955	rBV2	1235	392	0.00%	0.000%
51	10.637	2967	2969	2970	rBV2	760	368	0.00%	0.000%
52	10.710	2990	2992	2994	rBV2	1121	643	0.00%	0.000%
53	10.891	3046	3048	3052	rBV4	1206	710	0.00%	0.000%
54	11.000	3080	3082	3085	rBV4	822	548	0.00%	0.000%
55	11.045	3094	3096	3102	rBV5	862	659	0.00%	0.000%
56	11.071	3102	3104	3105	rBV2	1417	723	0.00%	0.000%
57	11.148	3125	3128	3129	rBV3	2080	1067	0.00%	0.000%
58	11.270	3155	3166	3185	rBV	747374	1139741	1.00%	0.444%
59	11.646	3271	3283	3301	rBV	748292	1156181	1.02%	0.450%
60	11.829	3337	3340	3341	rBV2	1850	1043	0.00%	0.000%
61	11.865	3347	3351	3353	rBV4	2247	1554	0.00%	0.001%
62	11.897	3357	3361	3364	rBV5	1249	1038	0.00%	0.000%
63	11.913	3364	3366	3368	rVV3	1002	437	0.00%	0.000%
64	11.958	3379	3380	3382	rBV3	942	463	0.00%	0.000%
65	12.038	3399	3405	3409	rBV6	2222	2799	0.00%	0.001%
66	12.099	3422	3424	3426	rBV2	890	406	0.00%	0.000%
67	12.173	3443	3447	3448	rBV4	1191	629	0.00%	0.000%
68	12.254	3469	3472	3473	rBV3	1308	743	0.00%	0.000%
69	12.337	3496	3498	3501	rVB4	1543	739	0.00%	0.000%
70	12.366	3501	3507	3511	rBV7	4595	5632	0.00%	0.002%
71	12.444	3529	3531	3535	rVB5	1020	676	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061920\
 Data File : VV017009.D
 Acq On : 19 Jun 2020 18:58
 Operator : SY/MD
 Sample : L3074-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.466	3535	3538	3542	rBV5	1560	1178	0.00%	0.000%
73	12.485	3542	3544	3545	rBV2	920	402	0.00%	0.000%
74	12.646	3591	3594	3598	rBV5	1423	1266	0.00%	0.000%
75	12.675	3598	3603	3605	rBV5	1916	1853	0.00%	0.001%
76	12.752	3623	3627	3629	rBV5	2178	1991	0.00%	0.001%
77	12.820	3646	3648	3650	rBV3	1455	916	0.00%	0.000%
78	13.025	3710	3712	3717	rVB4	1820	1223	0.00%	0.000%
79	13.061	3717	3723	3724	rBV4	1699	1278	0.00%	0.000%
80	13.228	3773	3775	3776	rBV2	968	437	0.00%	0.000%
81	13.260	3780	3785	3786	rBV4	1527	1383	0.00%	0.001%
82	13.373	3817	3820	3822	rBV4	1510	1000	0.00%	0.000%
83	13.614	3891	3895	3899	rBV6	1920	1481	0.00%	0.001%
84	13.746	3930	3936	3939	rBV8	1148	1124	0.00%	0.000%
85	13.868	3972	3974	3976	rVB3	1292	544	0.00%	0.000%
86	13.884	3976	3979	3981	rBV4	1169	926	0.00%	0.000%
87	13.916	3986	3989	3991	rBV4	1104	658	0.00%	0.000%
88	14.019	4018	4021	4024	rBV4	2035	1271	0.00%	0.000%
89	14.035	4024	4026	4032	rVB6	1385	1256	0.00%	0.000%
90	14.064	4032	4035	4036	rBV3	1089	548	0.00%	0.000%
91	14.408	4140	4142	4144	rBV2	1330	624	0.00%	0.000%
92	14.514	4173	4175	4176	rBV2	1040	384	0.00%	0.000%
93	14.569	4188	4192	4194	rBV3	1727	1001	0.00%	0.000%
94	14.768	4249	4254	4258	rBV7	2053	2222	0.00%	0.001%
95	14.800	4261	4264	4266	rBV3	2305	1346	0.00%	0.001%
96	14.878	4285	4288	4290	rBV4	1884	1241	0.00%	0.000%
97	15.099	4353	4357	4358	rBV4	916	454	0.00%	0.000%
98	15.128	4363	4366	4370	rBV5	1894	1103	0.00%	0.000%
99	15.398	4447	4450	4452	rBV4	1128	772	0.00%	0.000%
100	15.434	4457	4461	4467	rVV8	1460	1609	0.00%	0.001%


Sum of corrected areas: 256916658

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061920\
Data File : VV017009.D
Acq On : 19 Jun 2020 18:58
Operator : SY/MD
Sample : L3074-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M21

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

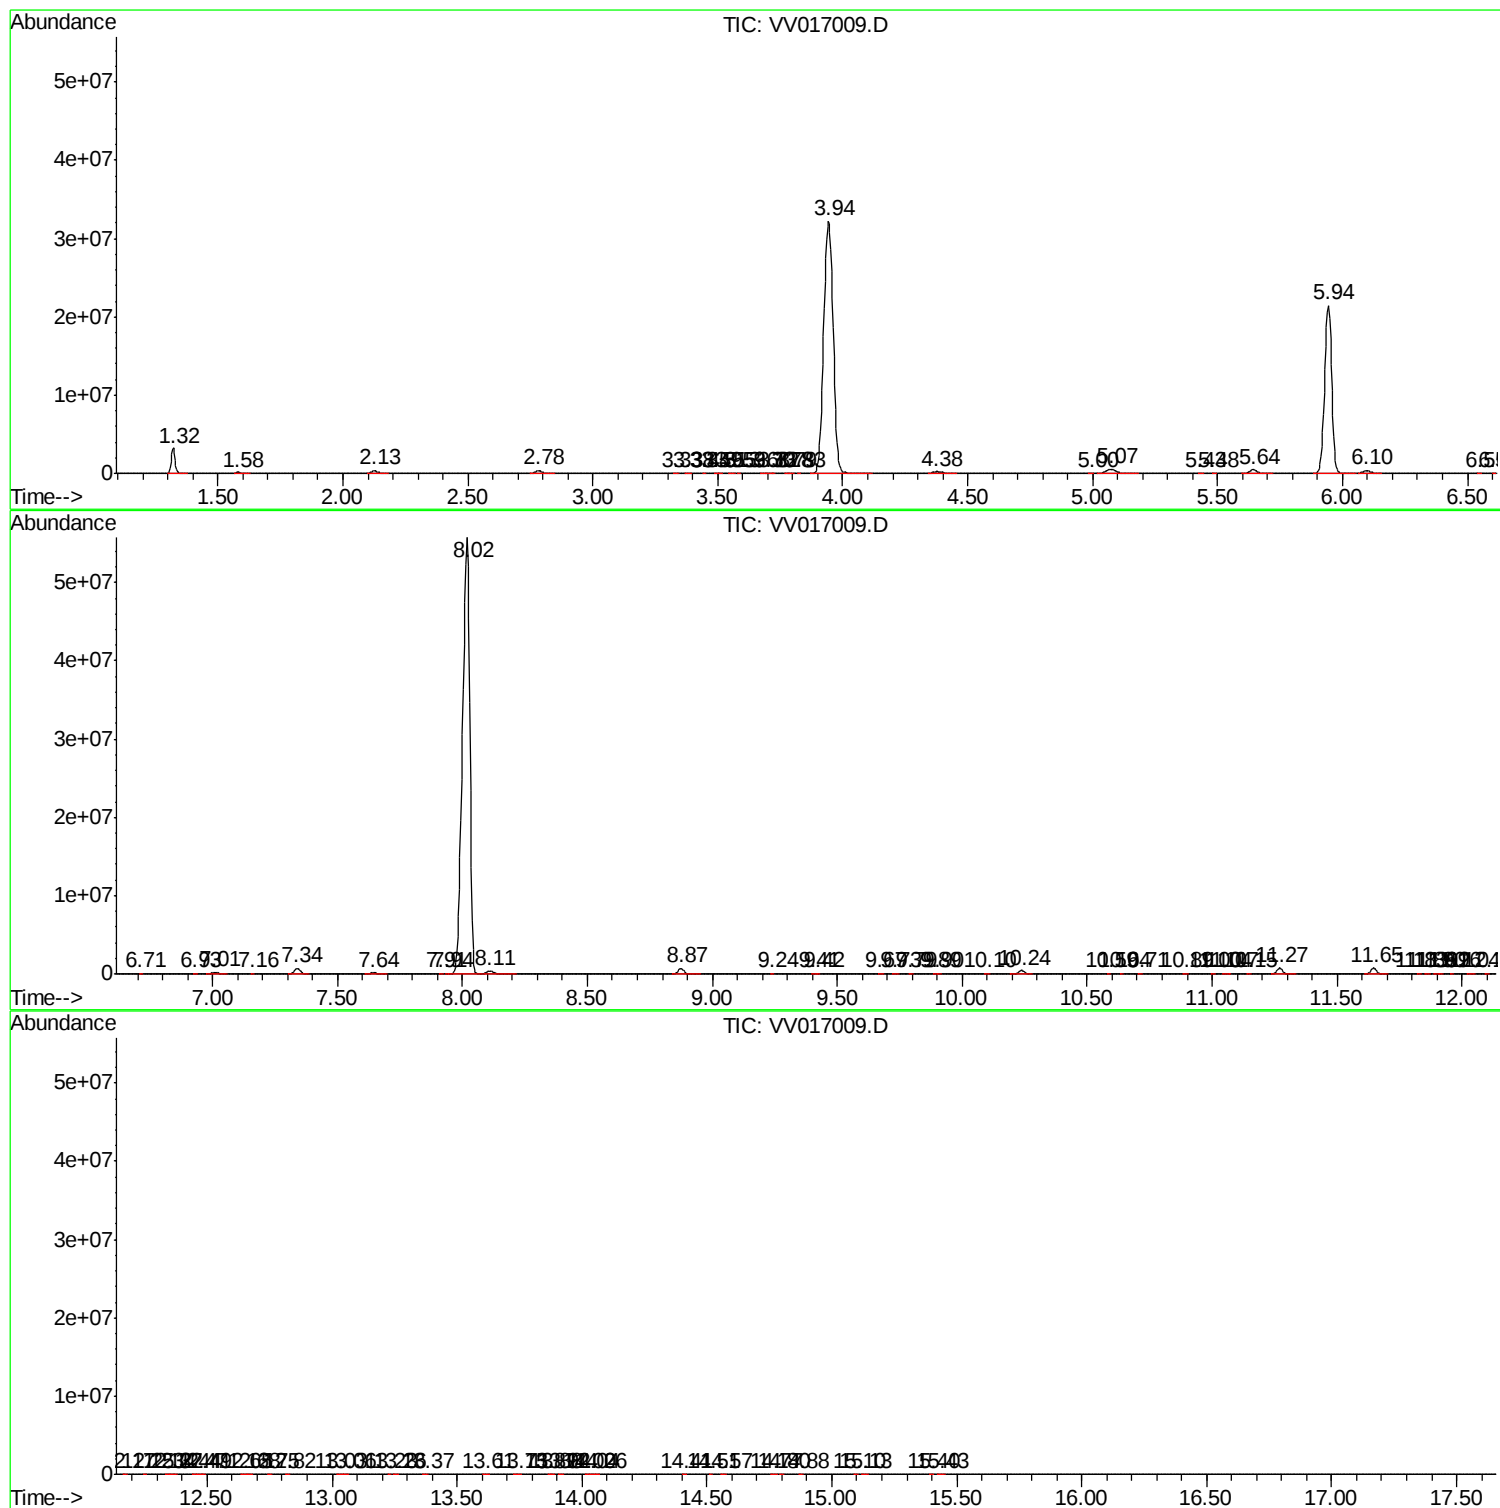

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017009.D
Acq On : 19 Jun 2020 18:58
Operator : SY/MD
Sample : L3074-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M21

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
Data File : VV017009.D
Acq On : 19 Jun 2020 18:58
Operator : SY/MD
Sample : L3074-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M21

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc