


Data Path : N:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061920\
 Data File : VV016990.D
 Acq On : 19 Jun 2020 08:59
 Operator : SY/MD
 Sample : BFB92
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB92

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Sat Jun 20 02:04:09 2020

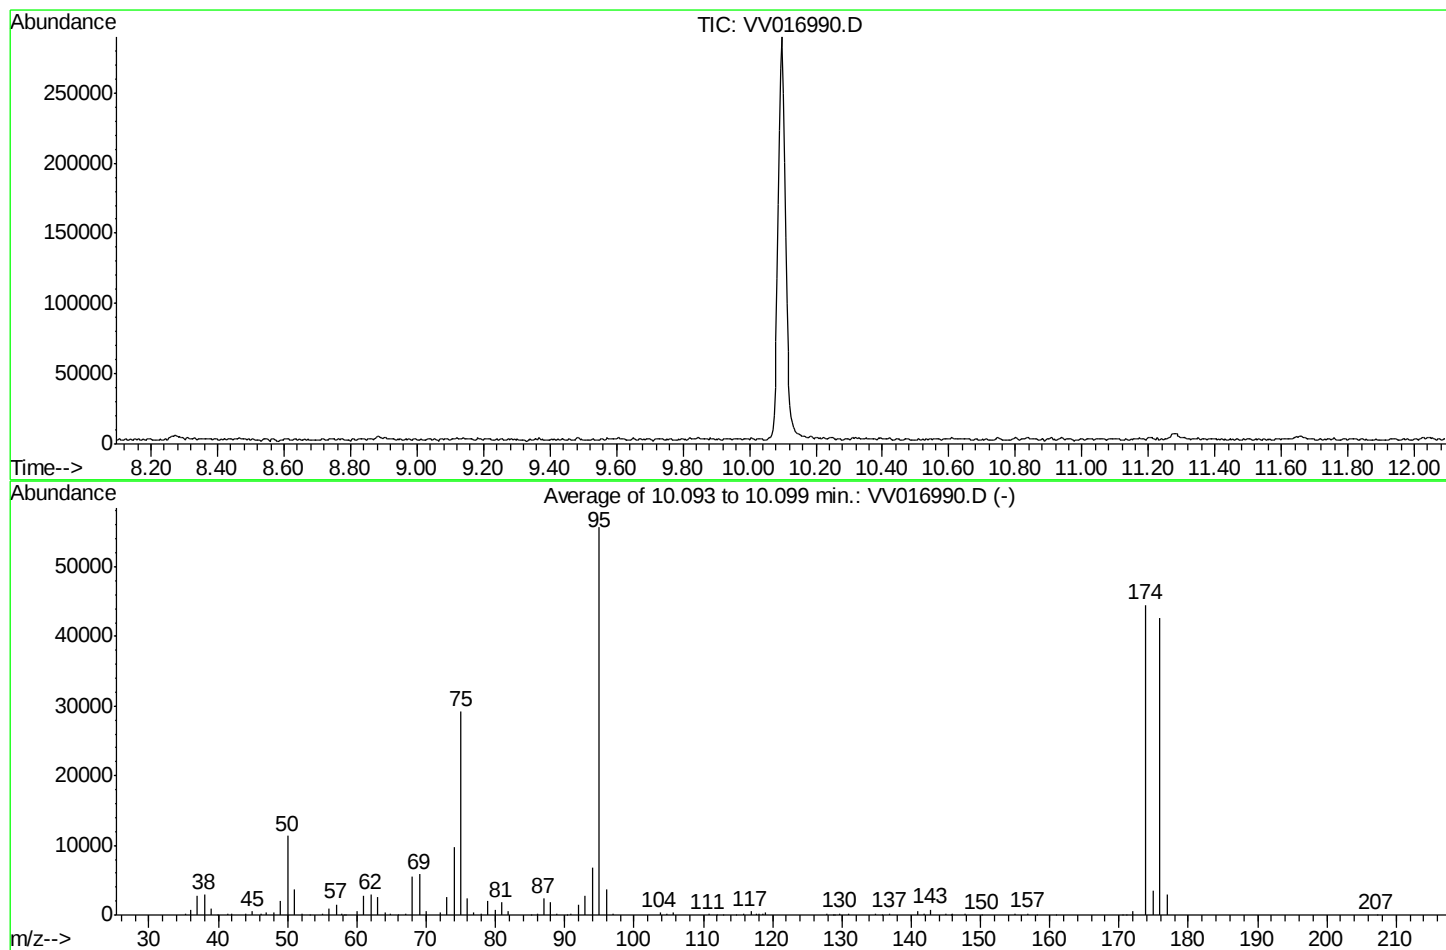

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	11322	PASS
75	95	30	80	52.4	29154	PASS
95	95	100	100	100.0	55669	PASS
96	95	5	9	6.7	3744	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	44490	PASS
175	174	5	9	7.8	3462	PASS
176	174	95	101	95.8	42613	PASS
177	176	5	9	7.1	3010	PASS

m/z	Abundance
36.00	155.0
37.70	116.0
38.40	121.0
38.90	150.0
40.00	303.0
41.00	145.0
41.10	145.0
42.10	141.0
43.10	156.0
44.00	474.0
46.90	180.0
47.60	103.0
48.40	129.0
49.20	131.0
51.20	122.0
53.20	114.0
59.00	122.0
62.30	124.0
64.70	193.0
68.70	103.0
71.20	126.0
73.70	167.0
75.80	154.0
76.60	115.0
84.30	112.0
98.60	145.0
106.10	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
35.30	109.0
36.00	836.0
37.00	2627.0
38.00	2964.0
39.00	971.0
40.00	347.0
41.00	136.0
41.40	119.0
41.80	109.0
43.90	721.0
45.00	464.0
46.20	148.0
47.00	698.0
48.00	449.0
49.00	2190.0
50.00	10935.0
51.00	3728.0
52.10	260.0
53.00	155.0
55.00	234.0
56.10	879.0
57.00	1522.0
57.90	243.0
60.00	512.0
61.00	2788.0
62.00	2900.0
63.00	2435.0
64.10	423.0
64.80	382.0
67.00	301.0
67.90	5259.0
69.00	5692.0
70.00	505.0
72.10	354.0
73.00	2532.0
74.00	9781.0
75.00	28096.0
76.00	2341.0
76.90	282.0
77.90	257.0
78.90	1830.0
79.90	813.0
80.90	1704.0
81.90	485.0
86.10	104.0
87.00	2222.0
87.90	1704.0
88.80	207.0
90.30	104.0
90.90	260.0
92.00	1402.0
93.00	2612.0
94.00	6376.0
95.00	52808.0
96.00	3664.0
96.90	203.0
103.80	264.0
104.70	132.0
105.80	356.0
110.80	113.0
111.90	109.0
115.70	171.0
116.90	488.0
117.70	210.0
118.10	215.0
118.90	403.0
127.80	226.0
128.70	136.0
129.80	230.0
130.90	113.0
134.80	151.0
136.90	172.0
140.90	612.0
141.90	126.0
142.80	858.0
145.00	222.0
145.70	130.0
147.70	185.0
154.90	153.0
156.80	155.0
158.10	107.0
160.80	104.0
170.50	161.0
171.80	484.0
173.90	42136.0
175.00	3477.0
175.90	39840.0
176.90	2936.0
207.30	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
35.30	130.0
36.00	900.0
37.00	2739.0
38.00	3015.0
39.00	1077.0
40.00	348.0
40.90	117.0
41.40	103.0
41.80	157.0
43.30	195.0
43.90	698.0
44.90	517.0
46.20	157.0
47.00	642.0
48.00	419.0
49.00	2230.0
50.00	11819.0
51.00	3968.0
52.10	268.0
53.10	174.0
55.00	266.0
56.00	818.0
57.00	1634.0
57.90	216.0
58.20	163.0
60.00	566.0
61.00	2842.0
62.00	2971.0
63.00	2647.0
64.10	490.0
64.90	500.0
65.90	113.0
67.00	266.0
67.90	5747.0
69.00	6040.0
70.00	489.0
71.30	115.0
72.10	361.0
73.00	2671.0
74.00	10192.0
75.00	30104.0
76.00	2608.0
76.90	400.0
78.00	249.0
78.90	2091.0
79.90	711.0
80.90	1835.0
81.90	585.0
85.20	117.0
86.10	123.0
87.00	2507.0
87.90	1848.0
88.80	219.0
90.90	232.0
92.00	1513.0
92.90	2788.0
94.00	7007.0
95.00	57720.0
96.00	3890.0
97.00	188.0
103.80	296.0
104.70	164.0
105.70	313.0
110.80	112.0
111.90	105.0
112.90	109.0
114.80	111.0
115.80	214.0
116.90	529.0
117.60	201.0
118.10	250.0
119.00	416.0
127.70	248.0
128.80	156.0
129.70	297.0
130.90	159.0
134.80	154.0
135.80	108.0
136.90	181.0
140.90	597.0
141.90	175.0
142.80	863.0
145.00	196.0
145.90	145.0
147.70	170.0
150.20	114.0
154.90	122.0
156.90	198.0
170.50	123.0
171.10	123.0
171.90	595.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

173.90	46024.0
175.00	3621.0
175.90	43896.0
176.90	3105.0
207.20	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

m/z	Abundance
35.30	129.0
36.00	924.0
37.00	2775.0
38.00	2679.0
39.00	1159.0
39.90	381.0
40.80	113.0
41.20	119.0
41.90	187.0
43.20	182.0
43.90	629.0
45.00	546.0
46.10	143.0
46.90	572.0
48.00	326.0
49.00	2172.0
50.00	11213.0
51.00	3691.0
52.10	248.0
53.10	169.0
55.00	279.0
55.90	836.0
57.00	1516.0
57.90	190.0
58.40	168.0
59.10	119.0
59.90	520.0
61.00	2602.0
62.00	2751.0
62.90	2434.0
64.10	440.0
64.90	520.0
65.90	146.0
67.00	202.0
68.00	5670.0
69.00	5834.0
70.00	467.0
71.20	153.0
72.00	340.0
73.00	2565.0
74.00	9270.0
75.00	29264.0
76.00	2531.0
76.90	483.0
78.90	2038.0
79.90	620.0
80.90	1886.0
81.80	607.0
85.20	137.0
86.10	148.0
87.00	2335.0
87.90	1941.0
88.80	172.0
90.90	212.0
92.00	1463.0
92.90	2682.0
94.00	6862.0
95.00	56480.0
96.00	3678.0
97.10	177.0
103.70	335.0
104.60	171.0
105.70	213.0
110.80	106.0
112.90	125.0
114.70	118.0
115.80	253.0
116.90	502.0
117.70	169.0
118.10	263.0
118.60	315.0
119.00	355.0
127.70	223.0
129.00	190.0
129.70	299.0
130.90	158.0
134.80	169.0
135.70	118.0
136.90	204.0
141.00	574.0
142.00	152.0
142.80	756.0
144.90	188.0
145.90	182.0
147.70	136.0
150.20	110.0
154.90	104.0
156.90	214.0
160.90	105.0
171.00	131.0
172.00	676.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92

173.90	45312.0
174.90	3290.0
175.90	44104.0
176.90	2989.0

Instrument :
MSVOA_V
ClientSampleId :
BFB92