

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031591.D
 Acq On : 19 Jun 2023 10:12
 Operator : SY/MD
 Sample : VV0619WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK359

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031591.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	40	44	51	rVB2	2259	2430	0.24%	0.033%
2	1.285	69	76	85	rBV	135649	142881	14.23%	1.920%
3	1.539	147	155	175	rVB	116838	143754	14.32%	1.932%
4	2.066	309	319	335	rBV	252114	365555	36.41%	4.913%
5	2.387	416	419	423	rVB2	288	233	0.02%	0.003%
6	2.455	434	440	451	rVV2	1457	2250	0.22%	0.030%
7	2.564	469	474	477	rBV2	220	305	0.03%	0.004%
8	2.783	535	542	545	rBV2	299	419	0.04%	0.006%
9	2.802	545	548	553	rVB	261	236	0.02%	0.003%
10	2.912	578	582	586	rBV3	334	297	0.03%	0.004%
11	2.934	586	589	595	rVB2	341	370	0.04%	0.005%
12	2.969	595	600	601	rBV	331	274	0.03%	0.004%
13	3.391	726	731	734	rBV2	260	233	0.02%	0.003%
14	3.410	734	737	743	rBV	274	335	0.03%	0.005%
15	3.439	743	746	749	rVV2	248	223	0.02%	0.003%
16	3.477	752	758	762	rBV2	341	416	0.04%	0.006%
17	3.558	777	783	787	rVV2	276	278	0.03%	0.004%
18	3.680	815	821	823	rBV2	293	353	0.04%	0.005%
19	3.722	831	834	843	rVB	369	387	0.04%	0.005%
20	3.799	847	858	896	rBV2	60929	173543	17.29%	2.332%
21	4.259	984	1001	1032	rBV2	159901	427493	42.58%	5.745%
22	4.542	1087	1089	1093	rVB3	598	468	0.05%	0.006%
23	4.966	1204	1221	1252	rBV2	378847	1003988	100.00%	13.494%
24	5.175	1284	1286	1290	rVB3	540	271	0.03%	0.004%
25	5.313	1325	1329	1333	rBV4	370	388	0.04%	0.005%
26	5.368	1341	1346	1348	rVB	327	259	0.03%	0.003%
27	5.387	1348	1352	1356	rBV2	266	333	0.03%	0.004%
28	5.429	1363	1365	1370	rVB2	289	272	0.03%	0.004%
29	5.542	1388	1400	1422	rBV	273784	563474	56.12%	7.573%
30	5.841	1483	1493	1506	rVB8	2352	5164	0.51%	0.069%
31	5.995	1528	1541	1577	rBV	225337	471040	46.92%	6.331%
32	6.201	1604	1605	1612	rVB3	327	322	0.03%	0.004%
33	6.448	1676	1682	1686	rBV3	366	403	0.04%	0.005%
34	6.715	1762	1765	1768	rVB	309	226	0.02%	0.003%
35	6.918	1818	1828	1870	rBV	106727	205984	20.52%	2.768%
36	7.120	1888	1891	1894	rBV	310	229	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031591.D
 Acq On : 19 Jun 2023 10:12
 Operator : SY/MD
 Sample : VV0619WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK359

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.136	1894	1896	1901	rVB3	473	216	0.02%	0.003%
38	7.181	1904	1910	1912	rBV3	249	255	0.03%	0.003%
39	7.249	1916	1931	1956	rBV	434186	758613	75.56%	10.196%
40	7.558	2017	2027	2057	rBV	85115	150332	14.97%	2.020%
41	7.770	2086	2093	2103	rBV3	290	533	0.05%	0.007%
42	8.030	2165	2174	2201	rBV	221838	395553	39.40%	5.316%
43	8.265	2244	2247	2251	rVB2	547	393	0.04%	0.005%
44	8.368	2271	2279	2288	rBV5	1659	2776	0.28%	0.037%
45	8.599	2345	2351	2355	rBV2	378	461	0.05%	0.006%
46	8.789	2399	2410	2438	rBV	441551	706819	70.40%	9.500%
47	9.088	2497	2503	2507	rBV3	383	403	0.04%	0.005%
48	9.204	2534	2539	2542	rVB	240	231	0.02%	0.003%
49	9.387	2594	2596	2600	rVB2	374	253	0.03%	0.003%
50	9.416	2600	2605	2607	rBV2	245	242	0.02%	0.003%
51	9.657	2677	2680	2687	rVB2	275	248	0.02%	0.003%
52	9.693	2687	2691	2697	rBV	339	323	0.03%	0.004%
53	9.805	2723	2726	2728	rVB2	400	228	0.02%	0.003%
54	9.834	2728	2735	2737	rBV2	261	328	0.03%	0.004%
55	10.027	2791	2795	2803	rVB3	622	846	0.08%	0.011%
56	10.159	2824	2836	2857	rBV	319363	501993	50.00%	6.747%
57	10.259	2863	2867	2869	rBV2	408	384	0.04%	0.005%
58	10.275	2869	2872	2875	rVV	380	252	0.03%	0.003%
59	10.329	2886	2889	2891	rBV2	360	223	0.02%	0.003%
60	10.378	2900	2904	2909	rBV	290	278	0.03%	0.004%
61	10.455	2925	2928	2932	rBV2	297	255	0.03%	0.003%
62	10.538	2950	2954	2957	rBV2	249	216	0.02%	0.003%
63	10.641	2981	2986	2989	rBV	255	268	0.03%	0.004%
64	10.850	3044	3051	3053	rBV2	468	531	0.05%	0.007%
65	11.043	3108	3111	3116	rVB	357	361	0.04%	0.005%
66	11.072	3116	3120	3122	rBV3	348	273	0.03%	0.004%
67	11.130	3132	3138	3146	rBV6	586	683	0.07%	0.009%
68	11.191	3146	3157	3181	rBV	439465	672198	66.95%	9.034%
69	11.439	3230	3234	3236	rBV2	322	282	0.03%	0.004%
70	11.567	3262	3274	3296	rVV	450496	708734	70.59%	9.525%
71	12.027	3411	3417	3420	rBV3	306	356	0.04%	0.005%
72	12.152	3450	3456	3458	rBV	325	335	0.03%	0.005%
73	12.197	3464	3470	3471	rBV2	839	638	0.06%	0.009%
74	12.287	3492	3498	3504	rBV2	503	552	0.05%	0.007%
75	12.535	3572	3575	3579	rVV	581	402	0.04%	0.005%
76	12.590	3588	3592	3600	rVB3	740	997	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031591.D
 Acq On : 19 Jun 2023 10:12
 Operator : SY/MD
 Sample : VV0619WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK359

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.721	3629	3633	3637	rVB2	274	234	0.02%	0.003%
78	12.744	3637	3640	3643	rBV2	334	272	0.03%	0.004%
79	12.844	3667	3671	3673	rBV	495	370	0.04%	0.005%
80	13.207	3780	3784	3791	rVV4	1318	1502	0.15%	0.020%
81	13.252	3795	3798	3804	rBV3	199	221	0.02%	0.003%
82	13.451	3852	3860	3870	rVV	3182	4820	0.48%	0.065%
83	13.561	3891	3894	3897	rBV2	336	256	0.03%	0.003%
84	13.599	3902	3906	3909	rBV2	395	261	0.03%	0.004%
85	13.689	3927	3934	3938	rBV4	1773	2138	0.21%	0.029%
86	13.863	3985	3988	3992	rVB4	420	342	0.03%	0.005%
87	13.972	4020	4022	4024	rBV	507	310	0.03%	0.004%
88	14.101	4057	4062	4064	rBV3	362	377	0.04%	0.005%
89	14.127	4068	4070	4074	rBV2	345	247	0.02%	0.003%
90	14.467	4170	4176	4178	rBV3	562	488	0.05%	0.007%
91	14.660	4233	4236	4238	rBV3	379	260	0.03%	0.003%
92	14.754	4262	4265	4271	rBV3	573	648	0.06%	0.009%
93	14.831	4287	4289	4295	rVB2	694	687	0.07%	0.009%
94	14.860	4295	4298	4300	rBV	508	410	0.04%	0.006%
95	15.056	4355	4359	4362	rBV2	561	579	0.06%	0.008%
96	15.098	4370	4372	4375	rBV	510	342	0.03%	0.005%
97	15.117	4375	4378	4381	rVV3	546	419	0.04%	0.006%
98	15.165	4391	4393	4395	rBV2	493	243	0.02%	0.003%
99	15.332	4441	4445	4448	rBV4	645	500	0.05%	0.007%
100	15.641	4539	4541	4542	rBV	558	250	0.02%	0.003%




Sum of corrected areas: 7440526

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031591.D
Acq On : 19 Jun 2023 10:12
Operator : SY/MD
Sample : VV0619WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK359

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

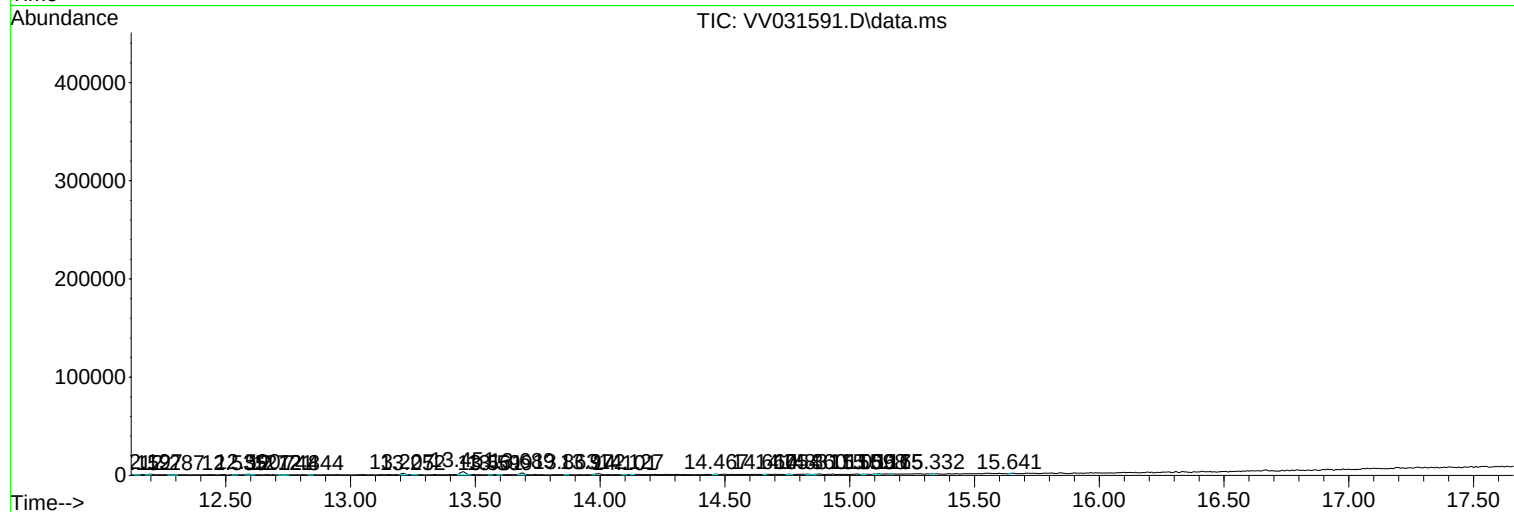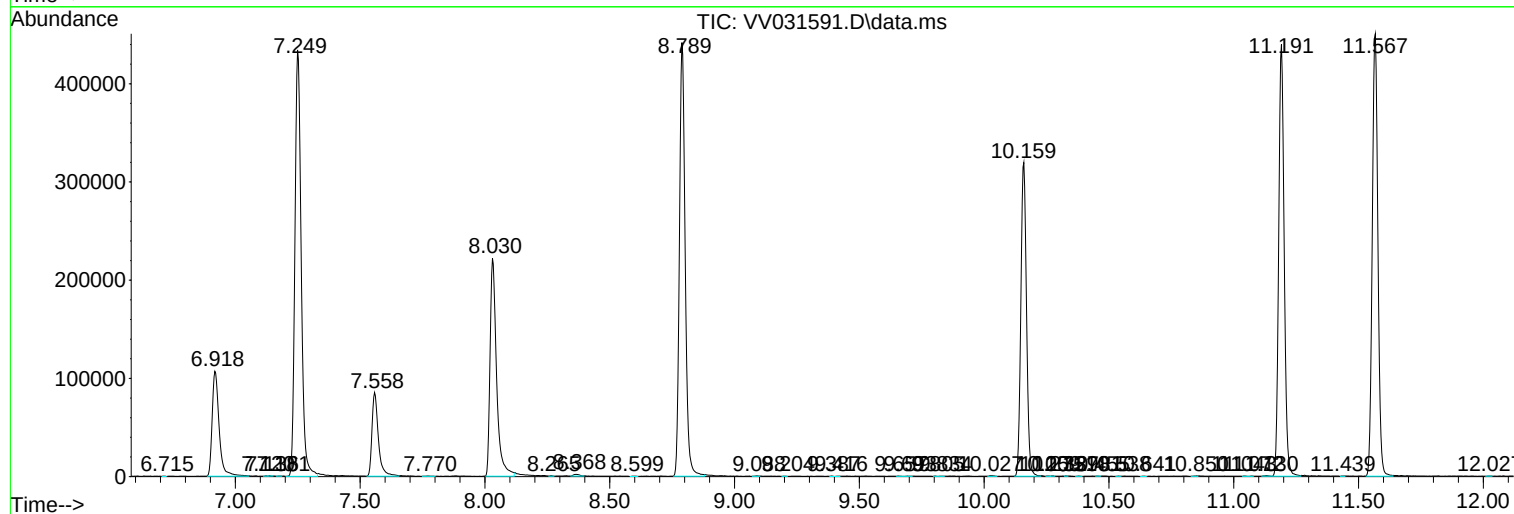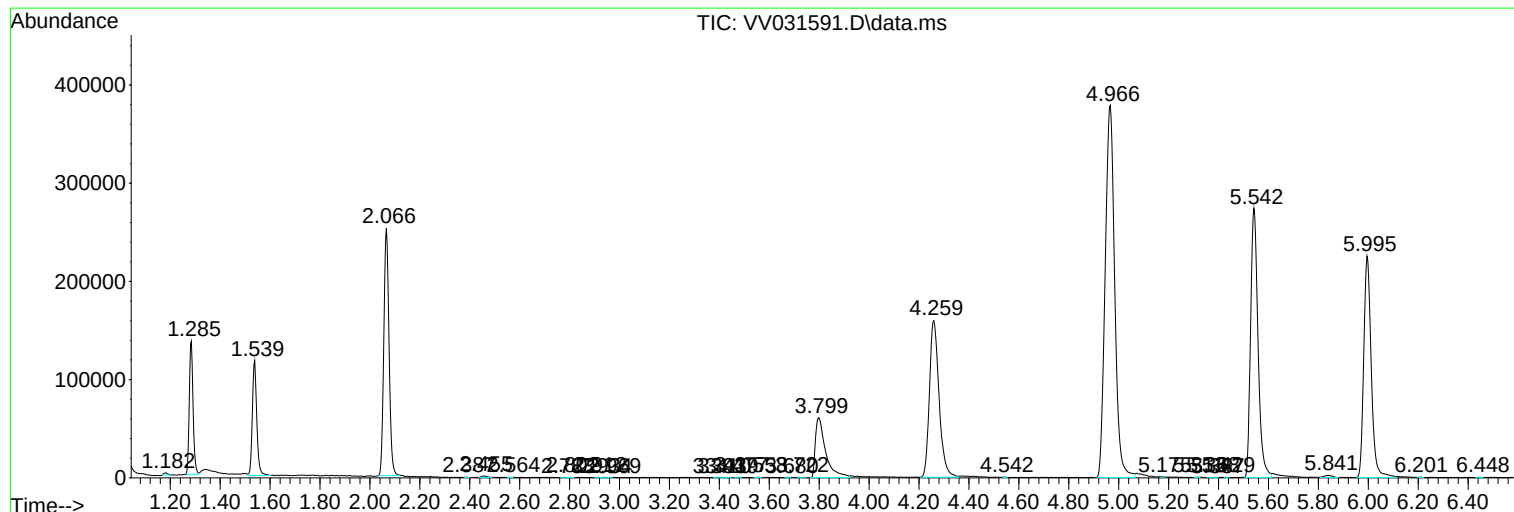

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031591.D
Acq On : 19 Jun 2023 10:12
Operator : SY/MD
Sample : VV0619WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK359

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031591.D
Acq On : 19 Jun 2023 10:12
Operator : SY/MD
Sample : VV0619WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK359

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------