

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031593.D
 Acq On : 19 Jun 2023 11:04
 Operator : SY/MD
 Sample : 03249-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rVB	132858	136389	13.97%	1.704%
2	1.535	147	154	167	rVB	113322	135860	13.91%	1.698%
3	2.066	308	319	334	rBV2	254526	387063	39.63%	4.837%
4	2.336	400	403	404	rBV	273	183	0.02%	0.002%
5	2.458	436	441	444	rBV3	714	713	0.07%	0.009%
6	2.529	457	463	464	rBV2	233	203	0.02%	0.003%
7	2.587	479	481	483	rVB	231	74	0.01%	0.001%
8	2.603	484	486	490	rVB2	231	152	0.02%	0.002%
9	2.645	496	499	500	rBV	236	163	0.02%	0.002%
10	2.709	508	519	531	rBV6	2612	4797	0.49%	0.060%
11	2.809	545	550	553	rBV	347	308	0.03%	0.004%
12	2.950	592	594	596	rBV2	190	123	0.01%	0.002%
13	2.989	604	606	608	rVB	257	118	0.01%	0.001%
14	3.008	608	612	615	rBV2	258	266	0.03%	0.003%
15	3.043	621	623	627	rVB	262	179	0.02%	0.002%
16	3.121	632	647	664	rBV	30064	62505	6.40%	0.781%
17	3.294	696	701	702	rBV2	254	216	0.02%	0.003%
18	3.352	715	719	721	rVB	148	97	0.01%	0.001%
19	3.375	722	726	729	rBV	286	228	0.02%	0.003%
20	3.416	736	739	740	rBV	194	113	0.01%	0.001%
21	3.510	765	768	772	rVB2	230	167	0.02%	0.002%
22	3.535	772	776	778	rBV	267	197	0.02%	0.002%
23	3.590	788	793	796	rVB	289	267	0.03%	0.003%
24	3.606	796	798	801	rVB	195	128	0.01%	0.002%
25	3.632	801	806	810	rBV2	299	303	0.03%	0.004%
26	3.715	830	832	835	rBV	185	119	0.01%	0.001%
27	3.744	838	841	844	rVB2	225	183	0.02%	0.002%
28	3.799	844	858	892	rBV	59368	189426	19.40%	2.367%
29	4.259	985	1001	1033	rBV	157006	414702	42.46%	5.182%
30	4.519	1064	1082	1107	rBV	224169	566735	58.03%	7.082%
31	4.805	1168	1171	1173	rBV2	241	185	0.02%	0.002%
32	4.963	1203	1220	1248	rBV2	366961	976600	100.00%	12.203%
33	5.281	1317	1319	1320	rBV2	303	102	0.01%	0.001%
34	5.313	1326	1329	1330	rBV	182	108	0.01%	0.001%
35	5.326	1330	1333	1338	rVB2	369	299	0.03%	0.004%
36	5.349	1338	1340	1341	rBV	184	58	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061923\
 Data File : VW031593.D
 Acq On : 19 Jun 2023 11:04
 Operator : SY/MD
 Sample : 03249-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.387	1347	1352	1353	rBV	330	305	0.03%	0.004%
38	5.458	1371	1374	1377	rBV	292	189	0.02%	0.002%
39	5.490	1381	1384	1387	rBV2	246	161	0.02%	0.002%
40	5.542	1387	1400	1426	rBV	270705	560257	57.37%	7.001%
41	5.770	1470	1471	1474	rBV2	365	193	0.02%	0.002%
42	5.802	1479	1481	1482	rBV2	266	92	0.01%	0.001%
43	5.844	1483	1494	1510	rVB6	12498	26112	2.67%	0.326%
44	5.905	1511	1513	1515	rBV	220	91	0.01%	0.001%
45	5.995	1526	1541	1563	rBV	219003	451464	46.23%	5.641%
46	6.230	1609	1614	1616	rBV2	334	265	0.03%	0.003%
47	6.291	1628	1633	1634	rBV2	336	190	0.02%	0.002%
48	6.452	1678	1683	1686	rVB2	356	272	0.03%	0.003%
49	6.500	1696	1698	1699	rBV	227	74	0.01%	0.001%
50	6.847	1802	1806	1809	rBV	241	224	0.02%	0.003%
51	6.918	1817	1828	1851	rBV	106294	197895	20.26%	2.473%
52	7.249	1918	1931	1964	rBV	415944	734448	75.20%	9.177%
53	7.558	2017	2027	2055	rBV	80649	147427	15.10%	1.842%
54	7.915	2117	2138	2154	rBV3	27779	58153	5.95%	0.727%
55	8.030	2162	2174	2204	rBV	212975	384441	39.37%	4.804%
56	8.432	2296	2299	2303	rBV	410	318	0.03%	0.004%
57	8.628	2358	2360	2362	rVB	238	60	0.01%	0.001%
58	8.789	2399	2410	2435	rBV	429928	700898	71.77%	8.758%
59	9.001	2473	2476	2479	rBV2	207	133	0.01%	0.002%
60	9.037	2486	2487	2490	rBV	229	135	0.01%	0.002%
61	9.095	2501	2505	2513	rVB4	446	476	0.05%	0.006%
62	9.149	2519	2522	2523	rBV	169	113	0.01%	0.001%
63	9.214	2539	2542	2544	rBV	155	84	0.01%	0.001%
64	9.429	2607	2609	2611	rVB	242	118	0.01%	0.001%
65	9.442	2611	2613	2614	rBV	253	107	0.01%	0.001%
66	9.895	2753	2754	2756	rBV	178	77	0.01%	0.001%
67	9.969	2774	2777	2778	rBV2	158	90	0.01%	0.001%
68	10.001	2782	2787	2789	rBV2	244	248	0.03%	0.003%
69	10.159	2824	2836	2863	rVB	307009	484920	49.65%	6.059%
70	10.329	2881	2889	2900	rVB2	7630	12081	1.24%	0.151%
71	10.403	2907	2912	2914	rBV	318	307	0.03%	0.004%
72	10.458	2926	2929	2933	rBV2	257	239	0.02%	0.003%
73	10.776	3027	3028	3035	rVB2	296	320	0.03%	0.004%
74	10.831	3035	3045	3049	rBV3	400	633	0.06%	0.008%
75	10.985	3089	3093	3095	rBV2	382	309	0.03%	0.004%
76	11.191	3146	3157	3180	rBV	431068	665201	68.11%	8.312%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031593.D
 Acq On : 19 Jun 2023 11:04
 Operator : SY/MD
 Sample : 03249-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

77	11.522	3257	3260	3262	rBV3	526	372	0.04%	0.005%
78	11.567	3262	3274	3296	rVV	439486	691815	70.84%	8.645%
79	12.136	3449	3451	3455	rBV	280	255	0.03%	0.003%
80	12.484	3554	3559	3564	rBV2	478	484	0.05%	0.006%
81	13.204	3780	3783	3789	rVB3	576	550	0.06%	0.007%
82	13.307	3813	3815	3817	rBV	368	177	0.02%	0.002%
83	13.673	3926	3929	3930	rBV2	416	215	0.02%	0.003%
84	14.207	4093	4095	4097	rBV2	519	209	0.02%	0.003%
85	14.496	4182	4185	4187	rBV	468	298	0.03%	0.004%




Sum of corrected areas: 8002824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031593.D
Acq On : 19 Jun 2023 11:04
Operator : SY/MD
Sample : 03249-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

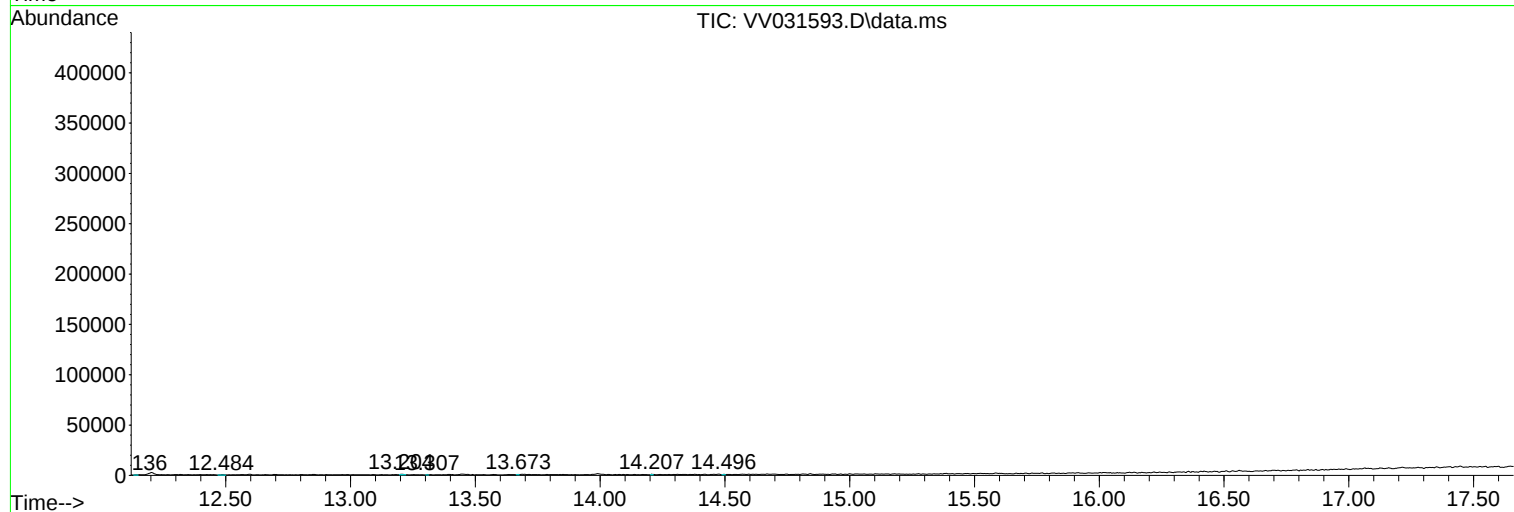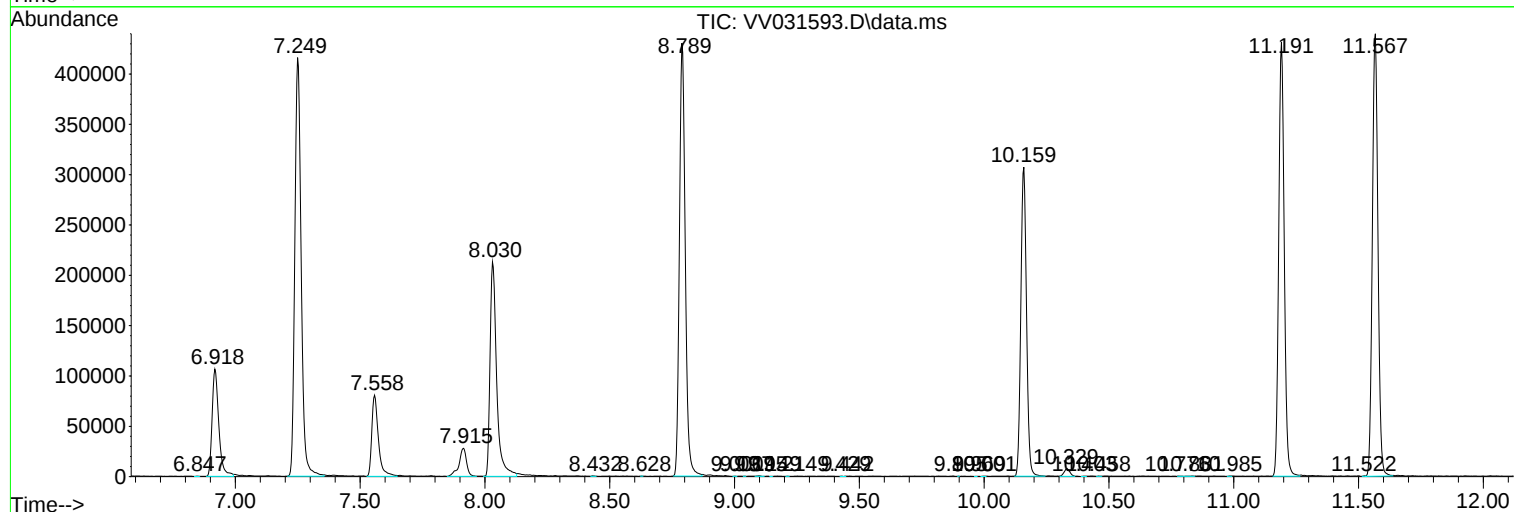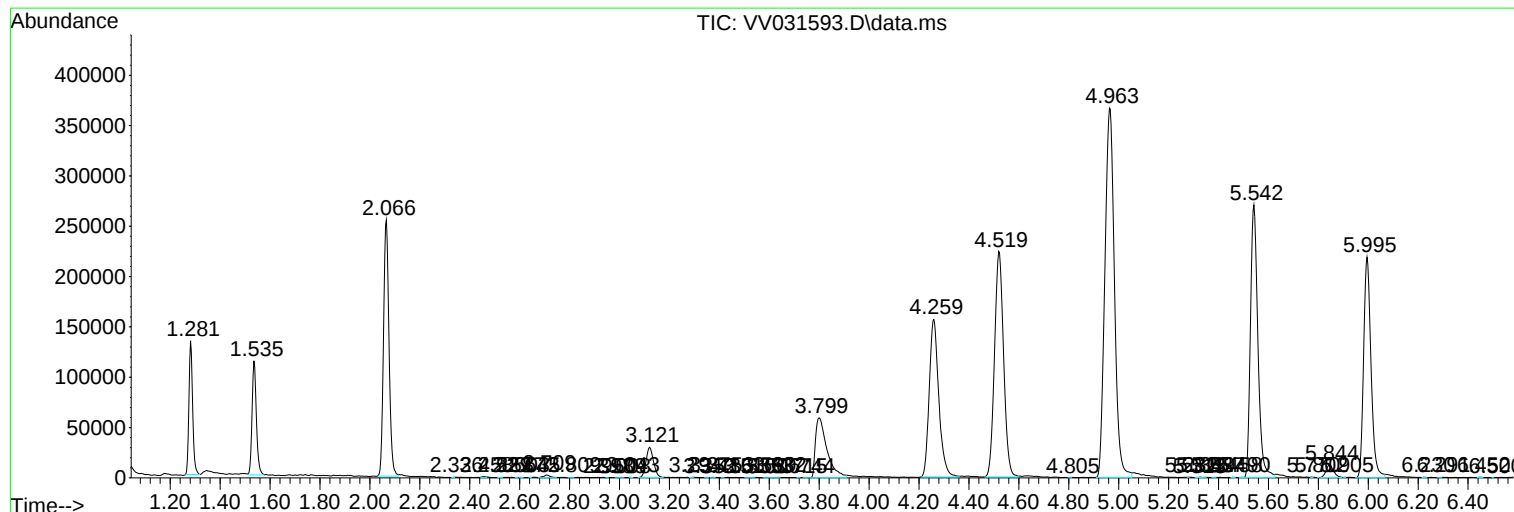

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031593.D
Acq On : 19 Jun 2023 11:04
Operator : SY/MD
Sample : 03249-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031593.D
Acq On : 19 Jun 2023 11:04
Operator : SY/MD
Sample : 03249-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc