

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031595.D
 Acq On : 19 Jun 2023 11:50
 Operator : SY/MD
 Sample : 03249-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	68	76	91	rVB2	181055	198589	21.53%	2.444%
2	1.536	147	154	171	rVB2	112265	194428	21.08%	2.393%
3	2.063	308	318	335	rBV	231674	342608	37.14%	4.216%
4	2.198	358	360	364	rBV3	398	288	0.03%	0.004%
5	2.420	425	429	433	rVB2	332	328	0.04%	0.004%
6	2.458	433	441	449	rBV5	2709	3870	0.42%	0.048%
7	2.571	472	476	477	rBV3	394	269	0.03%	0.003%
8	2.703	509	517	536	rVB3	7124	12848	1.39%	0.158%
9	2.780	536	541	545	rBV3	308	261	0.03%	0.003%
10	2.851	559	563	567	rBV2	315	267	0.03%	0.003%
11	2.925	582	586	592	rVB2	222	209	0.02%	0.003%
12	3.053	623	626	631	rBV	348	240	0.03%	0.003%
13	3.118	631	646	673	rBV	202415	424157	45.98%	5.220%
14	3.220	676	678	680	rBV	459	223	0.02%	0.003%
15	3.330	709	712	716	rVB3	314	208	0.02%	0.003%
16	3.674	815	819	826	rVB2	262	345	0.04%	0.004%
17	3.822	848	865	894	rBV3	190279	565990	61.35%	6.965%
18	4.111	952	955	958	rVB3	330	227	0.02%	0.003%
19	4.166	969	972	978	rVB2	308	274	0.03%	0.003%
20	4.259	983	1001	1030	rBV	145568	389293	42.20%	4.791%
21	4.519	1067	1082	1106	rVB	66335	168936	18.31%	2.079%
22	4.651	1118	1123	1124	rBV2	374	336	0.04%	0.004%
23	4.864	1184	1189	1193	rBV3	286	311	0.03%	0.004%
24	4.966	1203	1221	1244	rBV2	347605	922541	100.00%	11.353%
25	5.542	1387	1400	1429	rBV	268470	557567	60.44%	6.862%
26	5.847	1483	1495	1513	rVB7	10108	21854	2.37%	0.269%
27	5.995	1527	1541	1562	rBV	205640	423311	45.89%	5.210%
28	6.143	1583	1587	1591	rVB3	648	555	0.06%	0.007%
29	6.346	1647	1650	1654	rVB2	383	271	0.03%	0.003%
30	6.378	1654	1660	1667	rVB5	505	506	0.05%	0.006%
31	6.587	1721	1725	1729	rBV3	391	361	0.04%	0.004%
32	6.802	1786	1792	1796	rBV	305	347	0.04%	0.004%
33	6.841	1800	1804	1810	rVB2	218	212	0.02%	0.003%
34	6.918	1818	1828	1855	rBV	99399	186976	20.27%	2.301%
35	7.108	1884	1887	1889	rBV2	368	245	0.03%	0.003%
36	7.143	1895	1898	1903	rVB	551	390	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061923\
 Data File : VW031595.D
 Acq On : 19 Jun 2023 11:50
 Operator : SY/MD
 Sample : 03249-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.249	1916	1931	1955	rBV	389364	685999	74.36%	8.442%
38	7.558	2017	2027	2048	rBV	74087	133022	14.42%	1.637%
39	7.879	2117	2127	2129	rBV2	2121	2478	0.27%	0.030%
40	7.915	2133	2138	2151	rVB5	6999	11519	1.25%	0.142%
41	7.976	2151	2157	2159	rBV2	241	250	0.03%	0.003%
42	8.031	2165	2174	2205	rBV	197281	366381	39.71%	4.509%
43	8.211	2228	2230	2233	rVB2	696	400	0.04%	0.005%
44	8.503	2315	2321	2322	rBV2	286	257	0.03%	0.003%
45	8.580	2334	2345	2347	rBV3	296	360	0.04%	0.004%
46	8.654	2365	2368	2370	rBV2	285	215	0.02%	0.003%
47	8.789	2399	2410	2434	rBV	421114	688297	74.61%	8.471%
48	9.085	2499	2502	2504	rBV	361	237	0.03%	0.003%
49	9.098	2504	2506	2510	rVV4	422	271	0.03%	0.003%
50	9.198	2535	2537	2541	rVB	377	222	0.02%	0.003%
51	9.227	2541	2546	2548	rBV2	358	350	0.04%	0.004%
52	9.458	2616	2618	2622	rVB2	479	357	0.04%	0.004%
53	9.497	2622	2630	2631	rBV2	524	585	0.06%	0.007%
54	9.555	2643	2648	2651	rBV2	329	251	0.03%	0.003%
55	9.812	2723	2728	2731	rBV	325	292	0.03%	0.004%
56	9.883	2746	2750	2754	rBV2	267	233	0.03%	0.003%
57	9.953	2769	2772	2777	rBV2	326	332	0.04%	0.004%
58	10.159	2823	2836	2852	rBV	295858	463776	50.27%	5.707%
59	10.330	2883	2889	2900	rVB3	2333	3396	0.37%	0.042%
60	10.410	2912	2914	2919	rVV	321	228	0.02%	0.003%
61	10.487	2935	2938	2942	rVB2	571	363	0.04%	0.004%
62	10.686	2993	3000	3005	rVB4	553	733	0.08%	0.009%
63	10.863	3048	3055	3063	rVB6	1384	2197	0.24%	0.027%
64	11.191	3145	3157	3179	rBV	426508	660360	71.58%	8.127%
65	11.358	3207	3209	3211	rVB	433	219	0.02%	0.003%
66	11.397	3217	3221	3224	rBV2	345	320	0.03%	0.004%
67	11.471	3238	3244	3248	rVB3	789	885	0.10%	0.011%
68	11.567	3261	3274	3294	rBV	421919	652235	70.70%	8.027%
69	11.799	3344	3346	3350	rBV2	420	268	0.03%	0.003%
70	11.870	3358	3368	3380	rBV2	10288	15816	1.71%	0.195%
71	11.928	3383	3386	3393	rBV3	328	353	0.04%	0.004%
72	12.008	3407	3411	3414	rBV2	317	272	0.03%	0.003%
73	12.056	3423	3426	3428	rBV2	380	254	0.03%	0.003%
74	12.146	3451	3454	3459	rVB3	291	224	0.02%	0.003%
75	12.185	3463	3466	3467	rVV	429	278	0.03%	0.003%
76	12.201	3467	3471	3479	rVB4	1207	1460	0.16%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031595.D
 Acq On : 19 Jun 2023 11:50
 Operator : SY/MD
 Sample : 03249-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.243	3479	3484	3487	rBV	348	364	0.04%	0.004%
78	12.397	3529	3532	3536	rBV	379	244	0.03%	0.003%
79	12.532	3571	3574	3579	rVB	359	305	0.03%	0.004%
80	12.558	3579	3582	3589	rVB2	405	409	0.04%	0.005%
81	12.805	3656	3659	3665	rVB2	317	327	0.04%	0.004%
82	12.841	3665	3670	3673	rBV	326	282	0.03%	0.003%
83	12.860	3673	3676	3679	rBV2	394	241	0.03%	0.003%
84	13.210	3779	3785	3788	rBV2	349	397	0.04%	0.005%
85	13.445	3854	3858	3859	rBV2	691	431	0.05%	0.005%
86	13.641	3916	3919	3921	rBV2	304	224	0.02%	0.003%
87	13.693	3930	3935	3940	rBV3	639	526	0.06%	0.006%
88	13.995	4020	4029	4035	rVV2	1198	1668	0.18%	0.021%
89	14.050	4043	4046	4050	rBV2	273	262	0.03%	0.003%
90	14.191	4087	4090	4091	rBV3	380	255	0.03%	0.003%
91	14.275	4113	4116	4117	rBV2	556	285	0.03%	0.004%
92	14.326	4126	4132	4135	rBV4	547	572	0.06%	0.007%
93	14.355	4139	4141	4144	rVB2	501	273	0.03%	0.003%
94	14.635	4224	4228	4229	rBV	575	369	0.04%	0.005%
95	14.702	4245	4249	4251	rBV2	596	411	0.04%	0.005%
96	14.918	4313	4316	4320	rBV3	794	498	0.05%	0.006%
97	15.281	4426	4429	4432	rVB3	953	505	0.05%	0.006%
98	15.387	4459	4462	4465	rBV3	912	444	0.05%	0.005%
99	15.805	4590	4592	4596	rBB3	846	371	0.04%	0.005%
100	15.850	4604	4606	4610	rBV3	658	495	0.05%	0.006%


Sum of corrected areas: 8125744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031595.D
Acq On : 19 Jun 2023 11:50
Operator : SY/MD
Sample : 03249-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

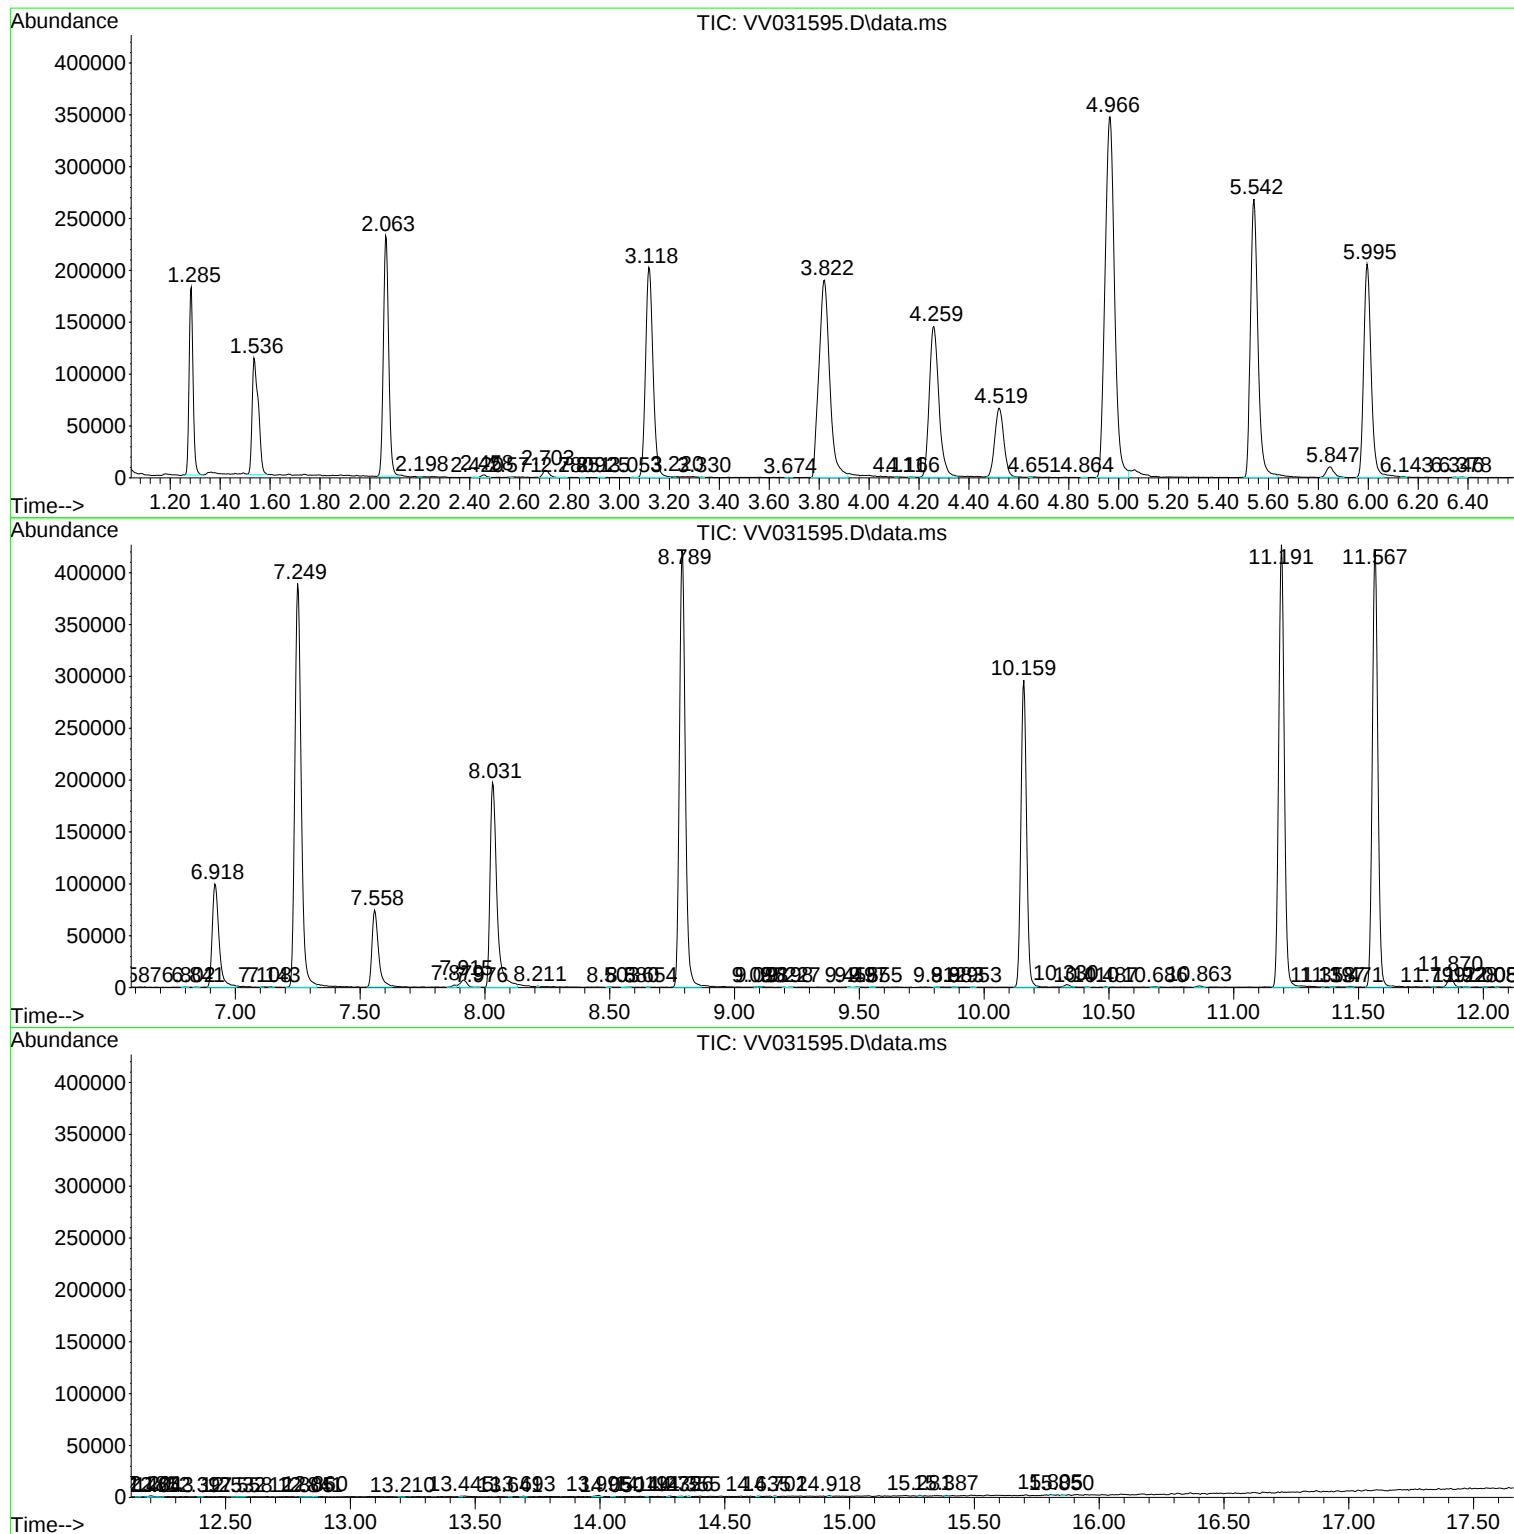

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031595.D
Acq On : 19 Jun 2023 11:50
Operator : SY/MD
Sample : 03249-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031595.D
Acq On : 19 Jun 2023 11:50
Operator : SY/MD
Sample : 03249-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------