

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031596.D
 Acq On : 19 Jun 2023 12:14
 Operator : SY/MD
 Sample : 03249-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	128349	134870	7.46%	1.456%
2	1.536	147	154	169	rVB	108864	127828	7.07%	1.380%
3	2.066	308	319	338	rBV2	248819	385222	21.32%	4.159%
4	2.240	370	373	375	rBV	408	315	0.02%	0.003%
5	2.410	423	426	431	rVB3	375	309	0.02%	0.003%
6	2.465	431	443	446	rBV6	926	1455	0.08%	0.016%
7	2.542	464	467	471	rVV3	437	405	0.02%	0.004%
8	2.603	484	486	490	rVB2	320	228	0.01%	0.002%
9	2.638	493	497	502	rBV2	372	352	0.02%	0.004%
10	2.703	508	517	534	rVB3	4744	8560	0.47%	0.092%
11	2.770	535	538	542	rVB	436	287	0.02%	0.003%
12	2.799	542	547	552	rBV2	299	396	0.02%	0.004%
13	2.934	583	589	591	rBV	286	324	0.02%	0.003%
14	2.986	602	605	611	rVB2	393	336	0.02%	0.004%
15	3.121	632	647	664	rBV2	75753	161204	8.92%	1.740%
16	3.236	681	683	689	rVB4	459	474	0.03%	0.005%
17	3.265	689	692	694	rBV	264	221	0.01%	0.002%
18	3.384	724	729	731	rBV	231	239	0.01%	0.003%
19	3.433	737	744	747	rBV	341	433	0.02%	0.005%
20	3.564	780	785	788	rBV2	320	254	0.01%	0.003%
21	3.732	834	837	841	rVB2	377	278	0.02%	0.003%
22	3.809	849	861	863	rBV	74964	123241	6.82%	1.331%
23	4.031	928	930	936	rVB2	450	318	0.02%	0.003%
24	4.259	984	1001	1033	rBV	147055	404039	22.36%	4.362%
25	4.519	1062	1082	1108	rBV	702129	1807009	100.00%	19.509%
26	4.825	1173	1177	1181	rBV2	515	328	0.02%	0.004%
27	4.860	1184	1188	1192	rVB2	265	230	0.01%	0.002%
28	4.966	1203	1221	1253	rBV2	355186	952087	52.69%	10.279%
29	5.223	1299	1301	1306	rVB2	415	224	0.01%	0.002%
30	5.542	1387	1400	1423	rBV	278031	566061	31.33%	6.111%
31	5.793	1475	1478	1481	rBV	310	240	0.01%	0.003%
32	5.847	1484	1495	1513	rVV7	13623	28895	1.60%	0.312%
33	5.995	1527	1541	1563	rBV	211135	433360	23.98%	4.679%
34	6.349	1646	1651	1654	rBV2	280	249	0.01%	0.003%
35	6.918	1817	1828	1851	rBV	103284	192691	10.66%	2.080%
36	7.117	1887	1890	1896	rBV2	354	375	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061923\
 Data File : VW031596.D
 Acq On : 19 Jun 2023 12:14
 Operator : SY/MD
 Sample : 03249-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.153	1897	1901	1906	rVB2	489	516	0.03%	0.006%
38	7.182	1907	1910	1913	rBV	404	244	0.01%	0.003%
39	7.249	1919	1931	1958	rBV	397384	696489	38.54%	7.520%
40	7.471	1998	2000	2006	rVB3	556	363	0.02%	0.004%
41	7.558	2014	2027	2055	rBV3	89667	171526	9.49%	1.852%
42	7.683	2064	2066	2070	rVB2	507	338	0.02%	0.004%
43	7.706	2070	2073	2077	rVV3	613	429	0.02%	0.005%
44	7.783	2091	2097	2106	rVB5	1396	1855	0.10%	0.020%
45	7.911	2118	2137	2158	rBV2	85423	150574	8.33%	1.626%
46	8.030	2164	2174	2211	rBV	205413	380809	21.07%	4.111%
47	8.223	2232	2234	2237	rBV3	360	258	0.01%	0.003%
48	8.374	2278	2281	2285	rBV2	320	275	0.02%	0.003%
49	8.622	2353	2358	2361	rBV3	293	284	0.02%	0.003%
50	8.789	2399	2410	2433	rBV	431057	698346	38.65%	7.540%
51	9.104	2504	2508	2513	rVV3	287	219	0.01%	0.002%
52	9.493	2625	2629	2633	rBV2	431	425	0.02%	0.005%
53	9.664	2679	2682	2685	rBV	307	233	0.01%	0.003%
54	9.747	2703	2708	2711	rVB2	333	260	0.01%	0.003%
55	9.792	2717	2722	2725	rBV2	358	400	0.02%	0.004%
56	9.873	2744	2747	2753	rVB3	293	269	0.01%	0.003%
57	9.940	2763	2768	2771	rBV	230	229	0.01%	0.002%
58	10.159	2824	2836	2861	rBV	302151	471508	26.09%	5.091%
59	10.265	2867	2869	2873	rVB3	445	263	0.01%	0.003%
60	10.336	2880	2891	2899	rVB4	2741	4043	0.22%	0.044%
61	10.429	2916	2920	2923	rBV2	262	228	0.01%	0.002%
62	10.564	2959	2962	2968	rBV2	444	385	0.02%	0.004%
63	10.921	3069	3073	3077	rBV2	368	339	0.02%	0.004%
64	10.976	3086	3090	3092	rBV2	341	259	0.01%	0.003%
65	11.133	3132	3139	3142	rVB3	324	387	0.02%	0.004%
66	11.191	3145	3157	3178	rBV	431751	667150	36.92%	7.203%
67	11.516	3251	3258	3260	rBV	343	396	0.02%	0.004%
68	11.567	3261	3274	3293	rVV	430599	666231	36.87%	7.193%
69	11.715	3318	3320	3322	rVB2	588	246	0.01%	0.003%
70	11.898	3374	3377	3382	rBV3	240	295	0.02%	0.003%
71	11.979	3398	3402	3404	rBV2	317	229	0.01%	0.002%
72	12.078	3428	3433	3435	rBV2	268	307	0.02%	0.003%
73	12.201	3461	3471	3478	rVB5	1167	1683	0.09%	0.018%
74	12.246	3478	3485	3487	rBV2	477	467	0.03%	0.005%
75	12.275	3491	3494	3497	rBV	421	332	0.02%	0.004%
76	12.371	3522	3524	3528	rVB2	456	310	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031596.D
 Acq On : 19 Jun 2023 12:14
 Operator : SY/MD
 Sample : 03249-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	12.731	3633	3636	3643	rVB3	318	316	0.02%	0.003%
78	12.767	3643	3647	3649	rBV2	302	295	0.02%	0.003%
79	13.066	3734	3740	3748	rBV3	409	616	0.03%	0.007%
80	13.146	3758	3765	3768	rBV2	482	484	0.03%	0.005%
81	13.185	3774	3777	3782	rVB2	319	267	0.01%	0.003%
82	13.210	3782	3785	3787	rBV3	366	281	0.02%	0.003%
83	13.252	3795	3798	3800	rBV3	345	226	0.01%	0.002%
84	13.484	3868	3870	3874	rVB2	346	245	0.01%	0.003%
85	13.615	3905	3911	3914	rBV3	295	327	0.02%	0.004%
86	13.718	3938	3943	3947	rBV2	352	475	0.03%	0.005%
87	13.985	4021	4026	4028	rBV2	781	713	0.04%	0.008%
88	14.053	4044	4047	4052	rVB3	512	375	0.02%	0.004%
89	14.085	4054	4057	4061	rBV2	356	354	0.02%	0.004%
90	14.152	4074	4078	4081	rBV2	583	489	0.03%	0.005%
91	14.271	4111	4115	4117	rBV2	597	398	0.02%	0.004%
92	14.316	4125	4129	4132	rBV2	427	314	0.02%	0.003%
93	14.766	4266	4269	4272	rBV2	413	348	0.02%	0.004%
94	14.789	4272	4276	4281	rVV5	750	707	0.04%	0.008%
95	14.927	4317	4319	4323	rBV4	429	330	0.02%	0.004%
96	15.053	4356	4358	4361	rBV	444	265	0.01%	0.003%
97	15.104	4370	4374	4377	rBV3	543	521	0.03%	0.006%
98	15.410	4467	4469	4471	rBV3	578	222	0.01%	0.002%
99	15.792	4586	4588	4591	rBV3	606	316	0.02%	0.003%
100	16.316	4749	4751	4754	rBV3	1088	630	0.03%	0.007%


Sum of corrected areas: 9262250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031596.D
Acq On : 19 Jun 2023 12:14
Operator : SY/MD
Sample : 03249-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

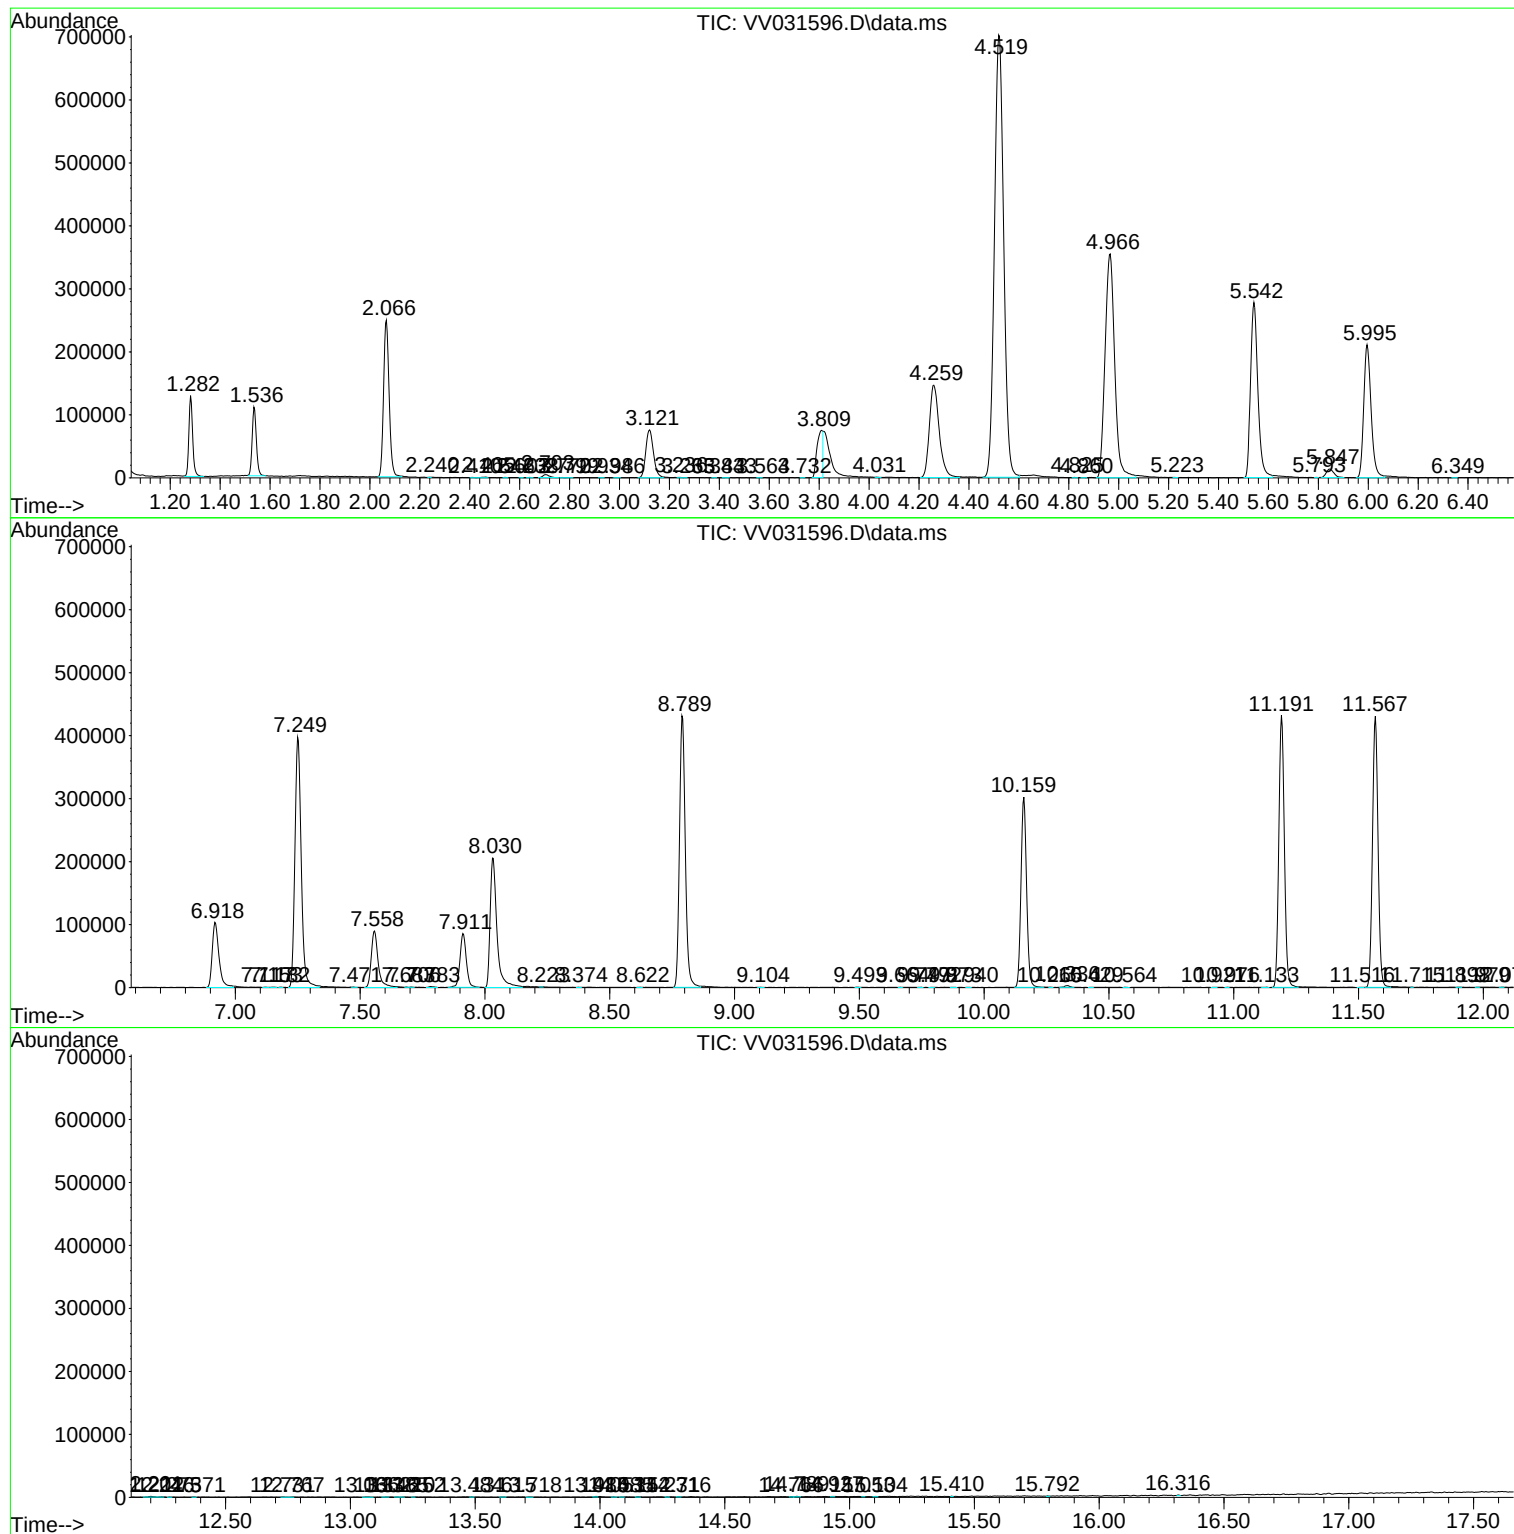

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031596.D
Acq On : 19 Jun 2023 12:14
Operator : SY/MD
Sample : 03249-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031596.D
Acq On : 19 Jun 2023 12:14
Operator : SY/MD
Sample : 03249-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc