

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031597.D
 Acq On : 19 Jun 2023 12:37
 Operator : SY/MD
 Sample : 03249-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	116148	120743	13.36%	1.844%
2	1.536	147	154	170	rVB	102641	122292	13.54%	1.867%
3	2.063	309	318	332	rBV	210352	302678	33.50%	4.622%
4	2.304	388	393	396	rBV4	273	235	0.03%	0.004%
5	2.323	397	399	401	rBV2	321	147	0.02%	0.002%
6	2.339	401	404	407	rVV	302	194	0.02%	0.003%
7	2.455	433	440	453	rVB3	2693	4185	0.46%	0.064%
8	2.565	472	474	477	rVB2	291	141	0.02%	0.002%
9	2.667	504	506	509	rVB	148	65	0.01%	0.001%
10	2.683	509	511	512	rBV	184	74	0.01%	0.001%
11	2.693	512	514	516	rVV	182	81	0.01%	0.001%
12	2.738	526	528	531	rBV	129	96	0.01%	0.001%
13	2.825	548	555	557	rBV2	385	435	0.05%	0.007%
14	3.076	631	633	634	rBV	84	31	0.00%	0.000%
15	3.101	639	641	643	rVB	227	98	0.01%	0.001%
16	3.285	691	698	699	rBV2	254	281	0.03%	0.004%
17	3.359	716	721	724	rBV2	246	276	0.03%	0.004%
18	3.394	729	732	733	rBV2	315	155	0.02%	0.002%
19	3.407	733	736	737	rBV	94	61	0.01%	0.001%
20	3.465	751	754	758	rBV	158	146	0.02%	0.002%
21	3.539	775	777	780	rBV	192	167	0.02%	0.003%
22	3.629	801	805	807	rBV	104	56	0.01%	0.001%
23	3.648	807	811	813	rBV	226	194	0.02%	0.003%
24	3.748	838	842	846	rBV2	364	434	0.05%	0.007%
25	3.799	848	858	882	rBV2	59468	163544	18.10%	2.497%
26	4.259	985	1001	1031	rBV	143910	384077	42.51%	5.864%
27	4.577	1097	1100	1108	rVB2	650	585	0.06%	0.009%
28	4.609	1108	1110	1112	rBV	141	105	0.01%	0.002%
29	4.642	1117	1120	1123	rBV2	240	141	0.02%	0.002%
30	4.693	1133	1136	1142	rVB	291	214	0.02%	0.003%
31	4.802	1168	1170	1174	rVB	421	263	0.03%	0.004%
32	4.825	1174	1177	1180	rBV	206	187	0.02%	0.003%
33	4.963	1203	1220	1246	rBV2	338550	903500	100.00%	13.795%
34	5.465	1374	1376	1379	rBV2	223	99	0.01%	0.002%
35	5.478	1379	1380	1381	rBV2	114	28	0.00%	0.000%
36	5.542	1387	1400	1430	rBV	235706	489096	54.13%	7.468%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
 Data File : VV031597.D
 Acq On : 19 Jun 2023 12:37
 Operator : SY/MD
 Sample : 03249-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.834	1485	1491	1497	rBV6	1542	2312	0.26%	0.035%
38	5.912	1512	1515	1518	rVB3	358	256	0.03%	0.004%
39	5.995	1528	1541	1564	rBV	206682	420158	46.50%	6.415%
40	6.272	1624	1627	1632	rBV2	317	323	0.04%	0.005%
41	6.388	1660	1663	1666	rBV	263	116	0.01%	0.002%
42	6.455	1682	1684	1688	rVB	248	110	0.01%	0.002%
43	6.529	1704	1707	1711	rBV2	195	149	0.02%	0.002%
44	6.699	1757	1760	1761	rBV	139	72	0.01%	0.001%
45	6.838	1798	1803	1807	rBV	319	350	0.04%	0.005%
46	6.918	1818	1828	1848	rBV	97876	180310	19.96%	2.753%
47	7.133	1892	1895	1899	rBV2	283	276	0.03%	0.004%
48	7.182	1907	1910	1911	rBV2	271	137	0.02%	0.002%
49	7.249	1919	1931	1958	rBV	368628	647830	71.70%	9.892%
50	7.558	2017	2027	2048	rBV	74714	134759	14.92%	2.058%
51	7.770	2091	2093	2094	rBV	257	94	0.01%	0.001%
52	8.031	2165	2174	2208	rBV	210281	386055	42.73%	5.895%
53	8.368	2272	2279	2289	rVB4	3233	4681	0.52%	0.071%
54	8.487	2313	2316	2319	rBV	377	261	0.03%	0.004%
55	8.510	2319	2323	2325	rBV2	198	197	0.02%	0.003%
56	8.744	2393	2396	2398	rBV2	213	126	0.01%	0.002%
57	8.789	2398	2410	2434	rBV	375891	610702	67.59%	9.325%
58	9.005	2473	2477	2480	rBV3	494	433	0.05%	0.007%
59	9.076	2496	2499	2501	rBV	189	134	0.01%	0.002%
60	9.127	2513	2515	2516	rBV	186	61	0.01%	0.001%
61	9.609	2662	2665	2669	rBV3	251	177	0.02%	0.003%
62	9.664	2679	2682	2684	rBV2	228	160	0.02%	0.002%
63	9.776	2714	2717	2718	rBV	299	145	0.02%	0.002%
64	10.159	2824	2836	2857	rBV	303321	474823	52.55%	7.250%
65	10.294	2876	2878	2880	rBV	160	54	0.01%	0.001%
66	10.487	2931	2938	2941	rBV3	486	537	0.06%	0.008%
67	11.191	3145	3157	3178	rBV	371602	574083	63.54%	8.766%
68	11.567	3261	3274	3293	rBV	394785	613062	67.85%	9.361%
69	12.394	3526	3531	3534	rBV2	368	410	0.05%	0.006%
70	12.882	3680	3683	3684	rBV	434	245	0.03%	0.004%
71	13.153	3764	3767	3769	rBV	352	233	0.03%	0.004%
72	13.378	3834	3837	3839	rBV2	291	223	0.02%	0.003%
73	13.953	4015	4016	4017	rBV2	473	153	0.02%	0.002%




Sum of corrected areas: 6549311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031597.D
Acq On : 19 Jun 2023 12:37
Operator : SY/MD
Sample : 03249-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

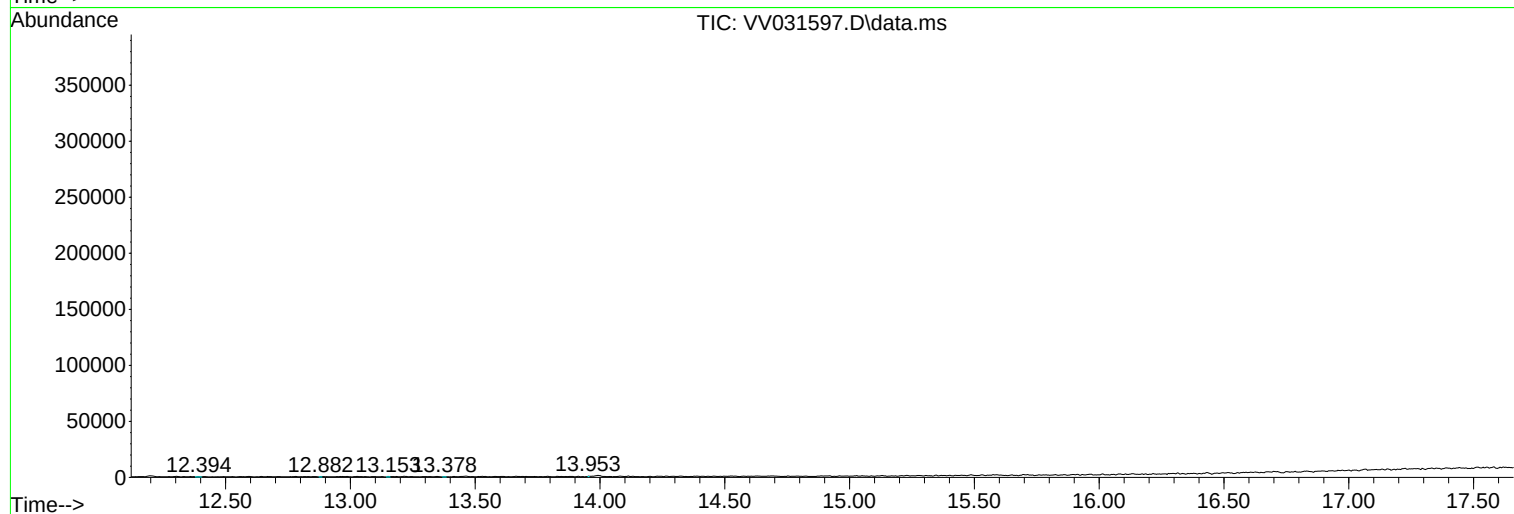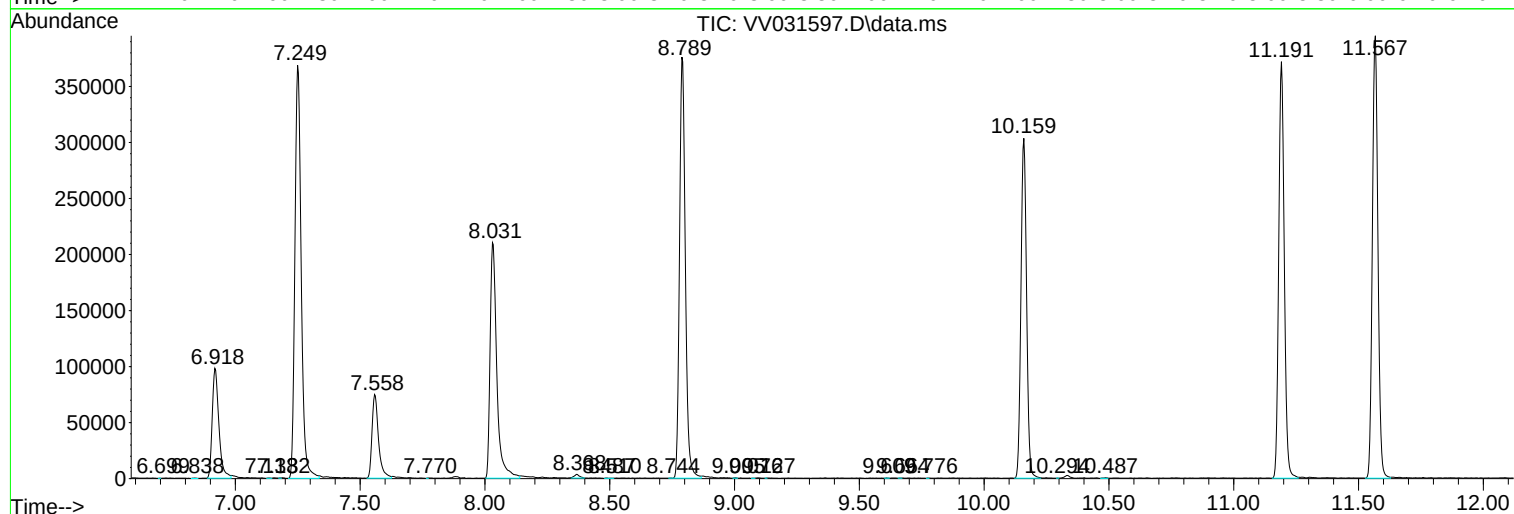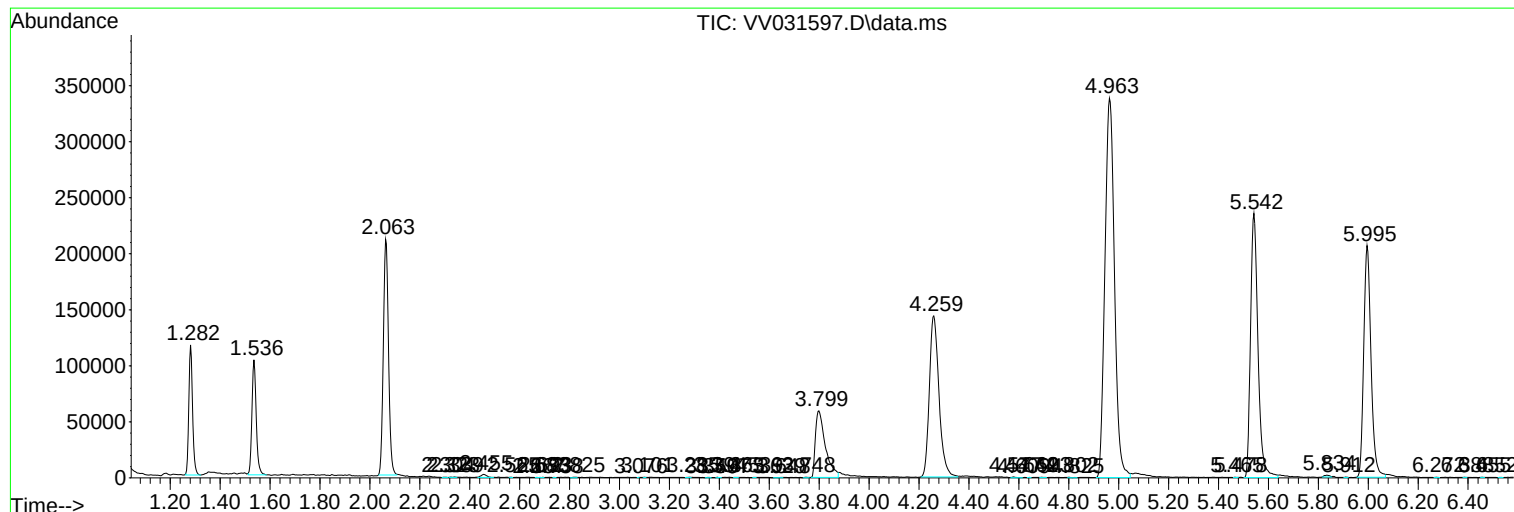

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031597.D
Acq On : 19 Jun 2023 12:37
Operator : SY/MD
Sample : 03249-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061923\
Data File : VV031597.D
Acq On : 19 Jun 2023 12:37
Operator : SY/MD
Sample : 03249-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------